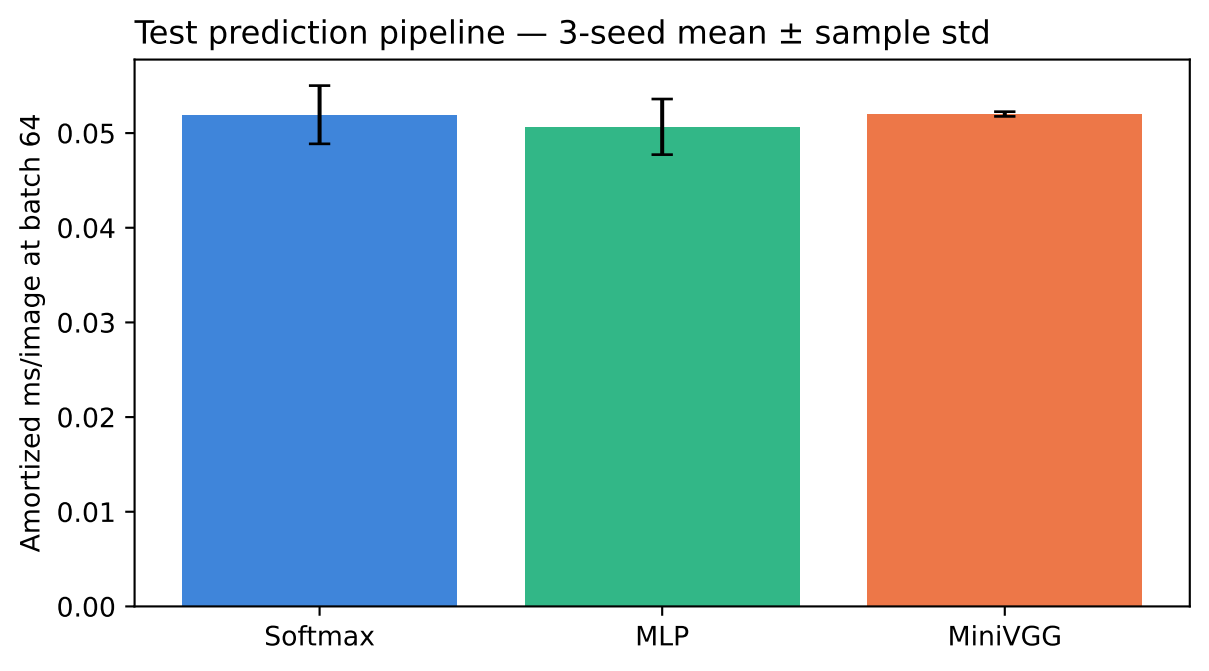
Test prediction pipeline — 3-seed mean ± sample std
Amortized ms/image at batch 64
0.00
0.01
0.02
0.03
0.04
0.05
Softmax
MLP
MiniVGG