


ITB 53-22 Surplus Laboratory and Maintenance Equipment - Exhibit C

ITEM 11: TS Dionex ICS-2100 with Dionex AS-AP System



ITEM 12: SEAL QuAAstro Continuous Segmented Flow Analyzer




ITEM 13: AT 7890B Gas Chromatograph and 5977A MSD



ITEM 14: TT Atomx Automated VOC Sample Preparation System




**ITEM 15: VS DK
Heating Digestor
42/26 Series**



ITEM 16: SEAL XY-2 Random Access Sampler



ITEM 17: PS Thelco Lab Oven, 130DM




ITEM 18: SEAL XY-2 Random Access Sampler





**ITEM 19: FS Precision Isotemp
GPD 20 Water Bath**

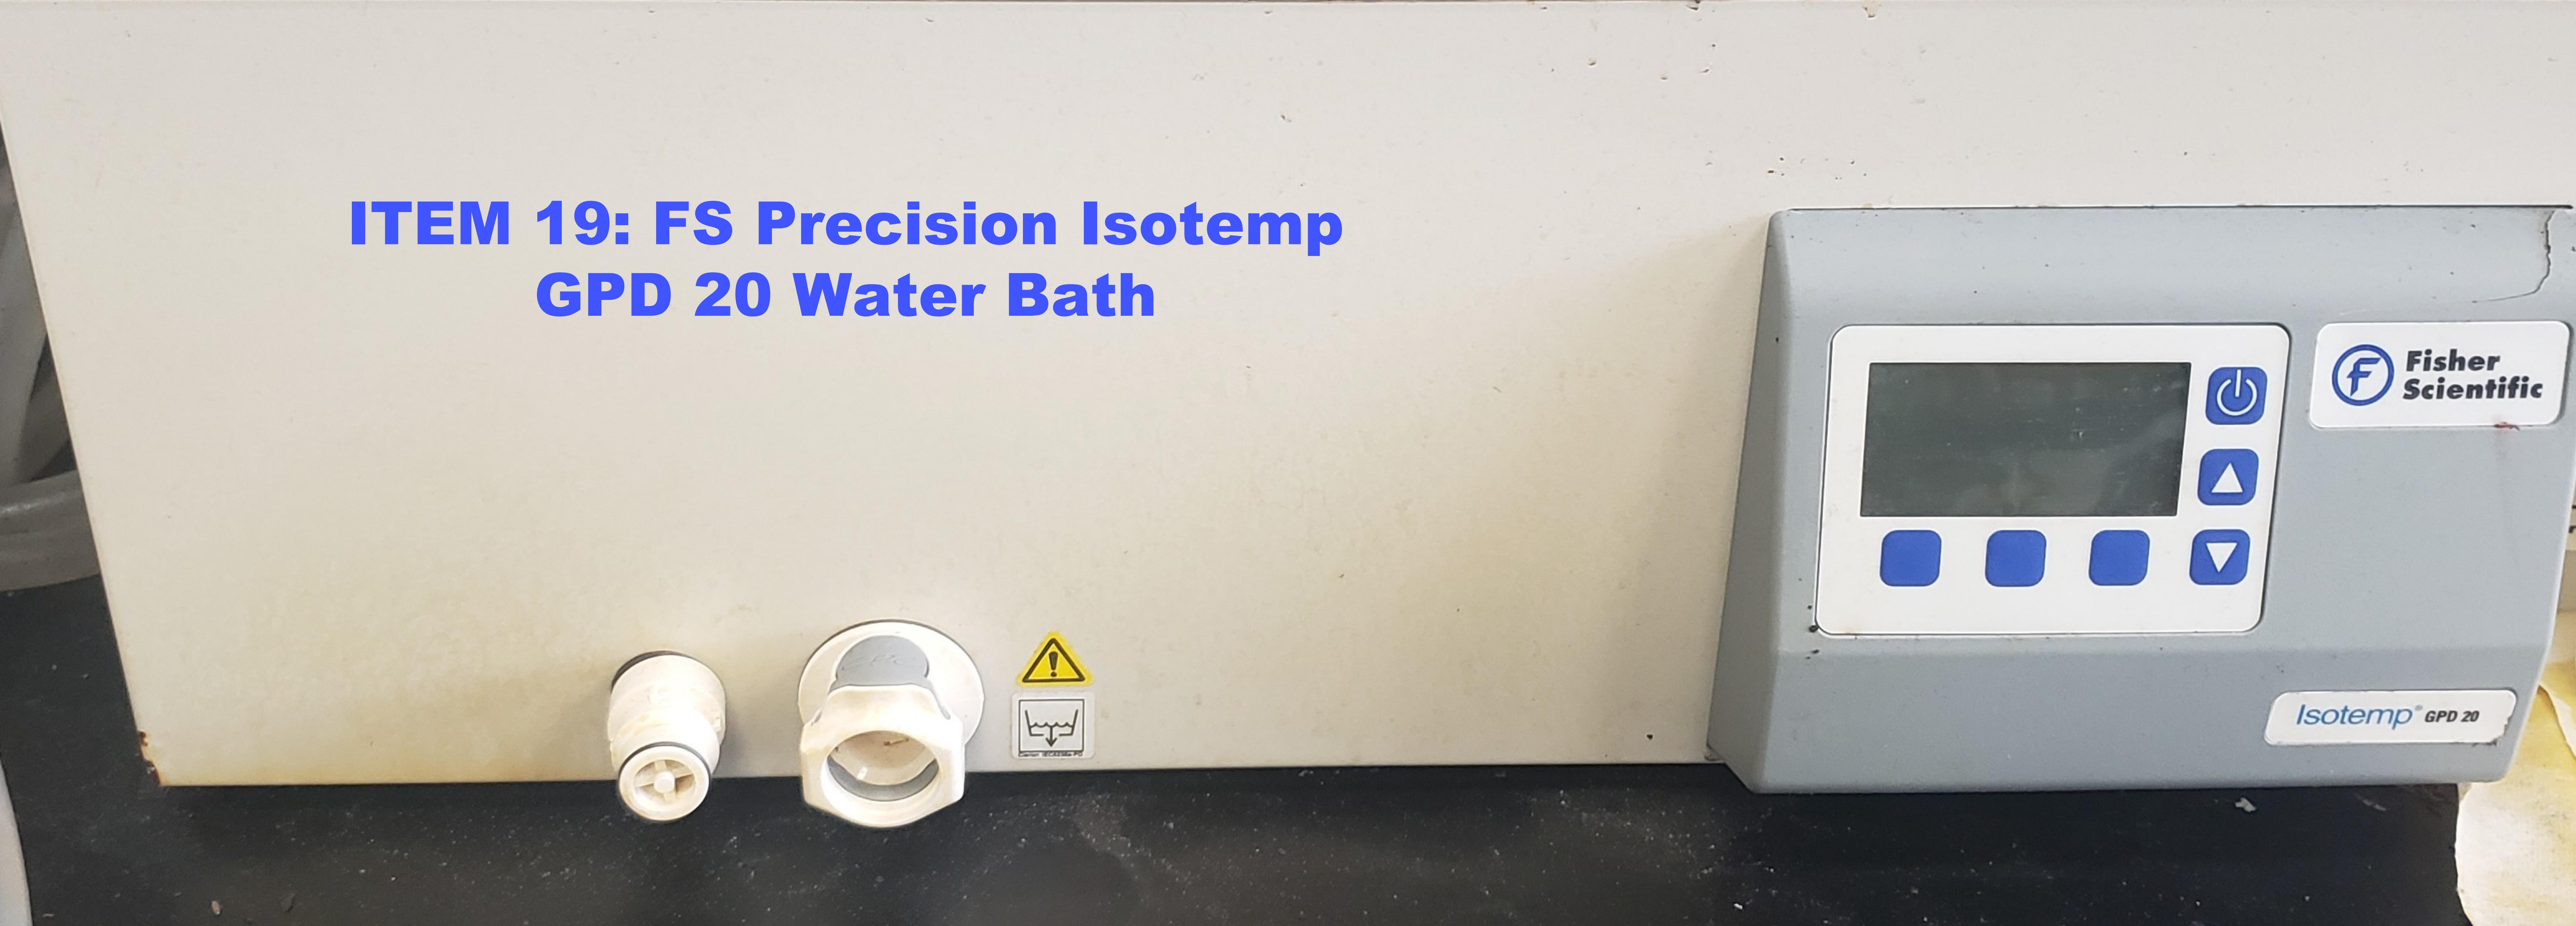

ITEM 20: TC DEENA Automated Sample Digestion System

Table 20-009
Eq. 20-009
Loc. Ref. 20-009

CITY OF CLEARWATER
City of Clearwater
#324655

Thomas Cain
A SEAL ANALYTICAL BRAND



DEENA

- DEENA
DIGESTION
BLOCK
OUT OF SERVICE
Since 7/16/2010

Please
Flush me
Before &
After //

