


Sample Name: VIT25-7118

```
=====
Acq. Operator   :                               Seq. Line :    2
Acq. Instrument : GC7890B                       Location  :    2
Injection Date  : 7/15/2025 15:50:40             Inj       :    1
                                                Inj Volume : 1 µl
Acq. Method     : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M
Last changed    : 7/15/2025 14:51:21
Analysis Method : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M (Sequence Method)
Last changed    : 7/16/2025 9:08:32
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

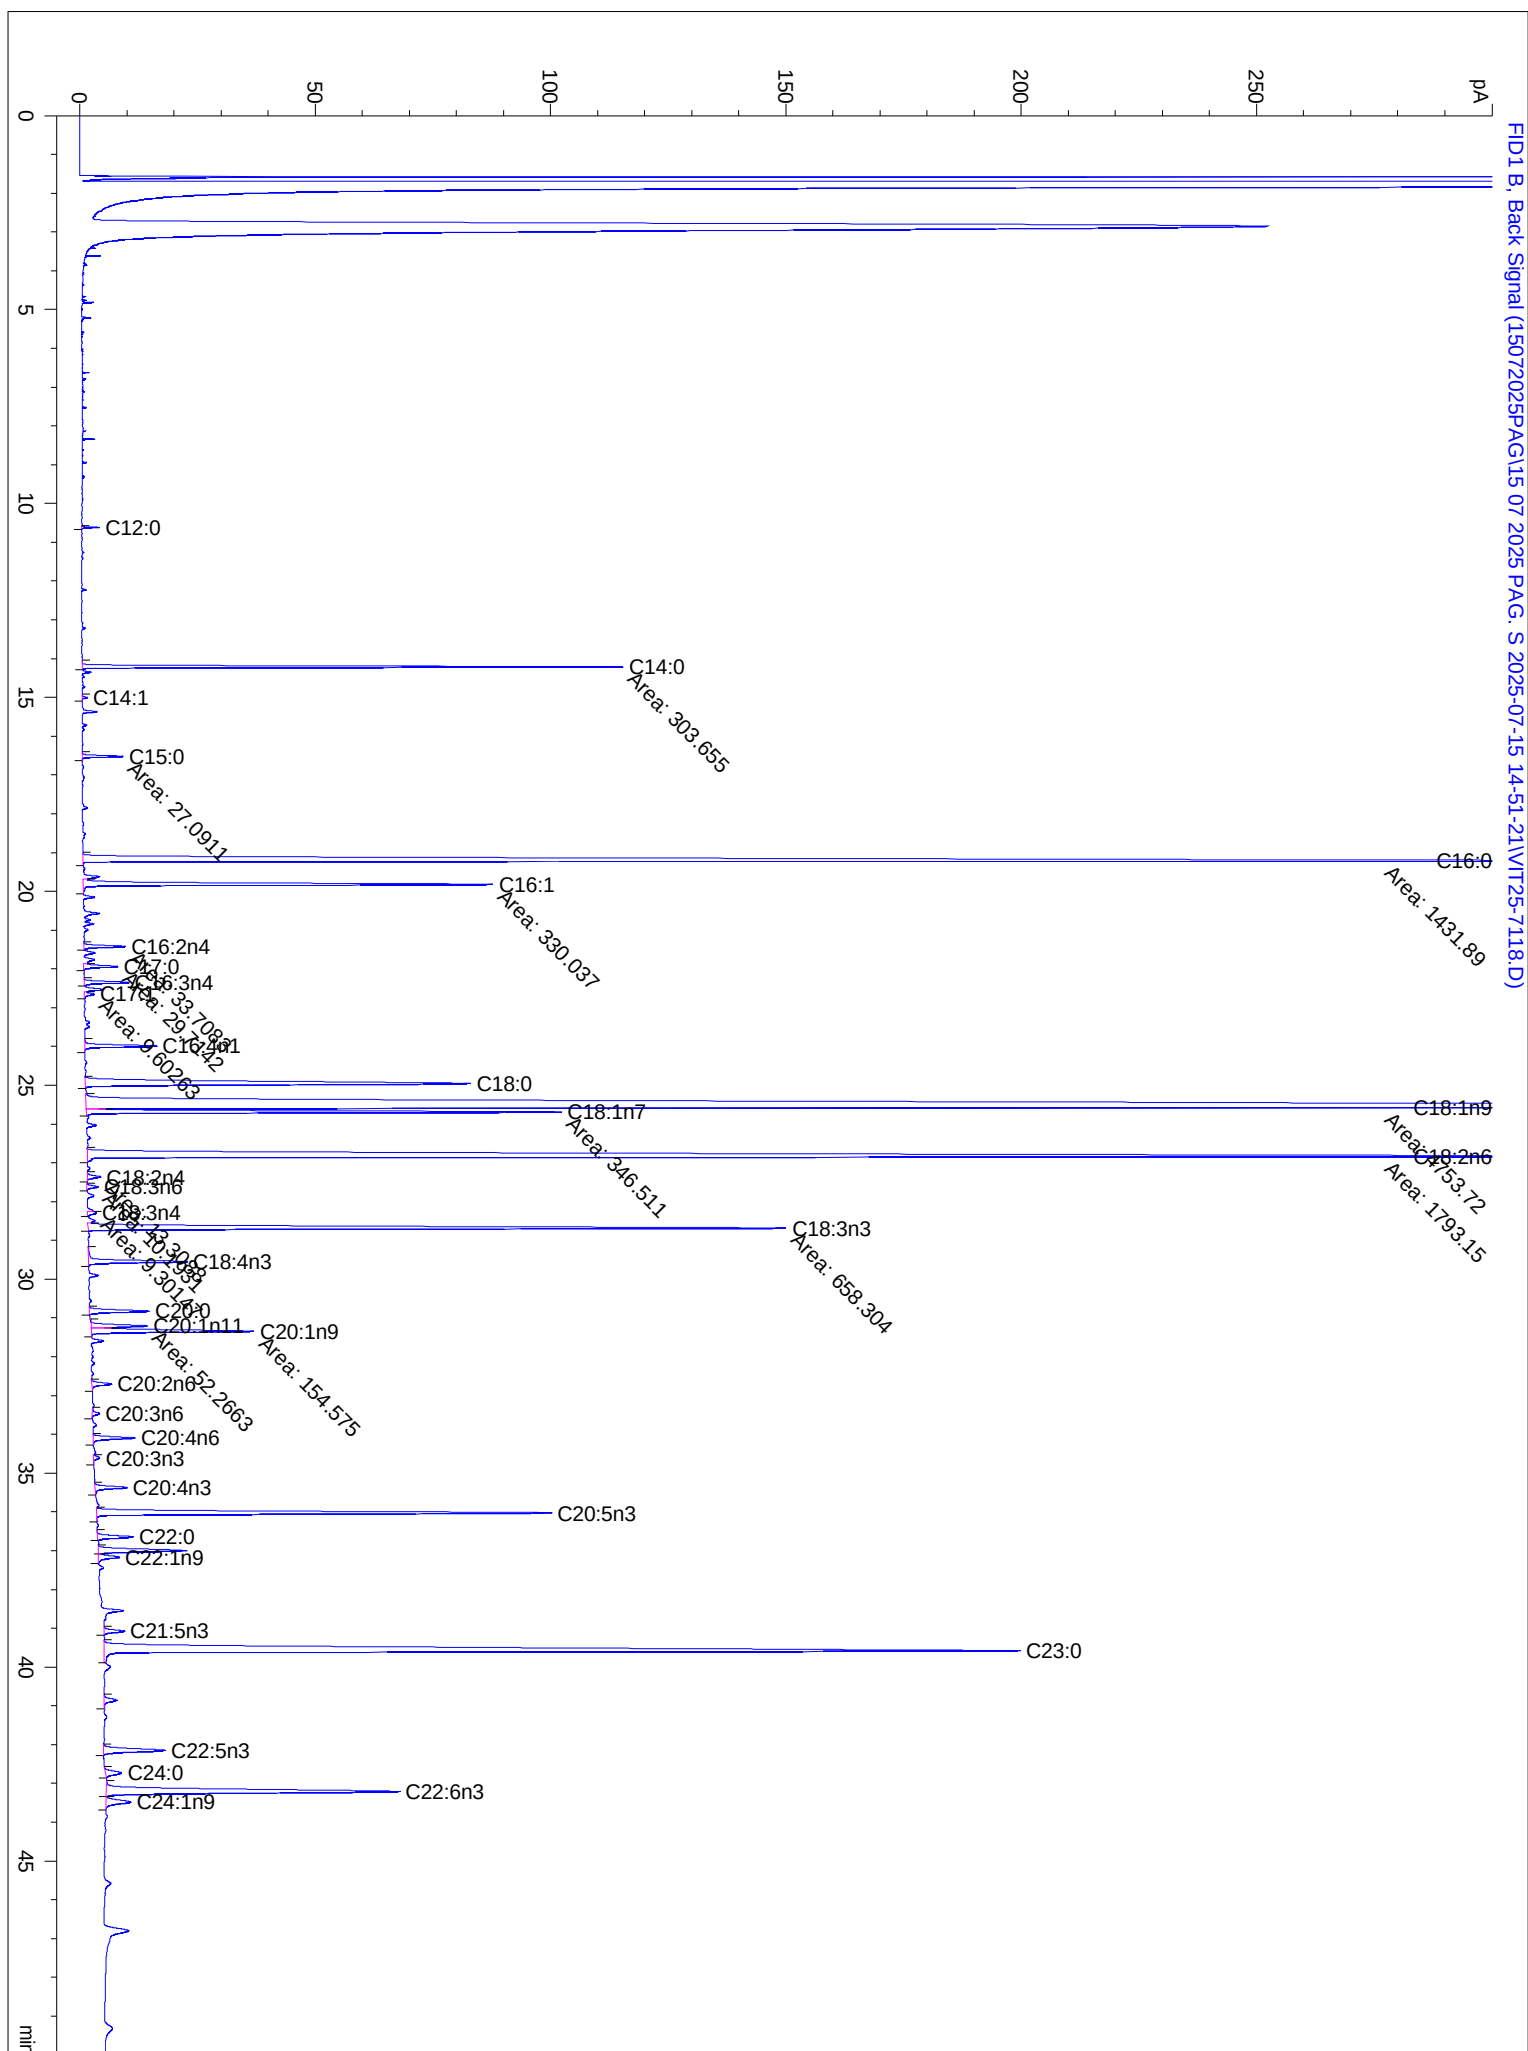

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 7/16/2025 9:08:31
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	0.000		0.0000	0.00000	0.00000	C18:2n6t
2	0.000		0.0000	0.00000	0.00000	C18:1n9t
3	3.450		0.0000	0.00000	0.00000	C4:0
4	5.255		0.0000	0.00000	0.00000	C6:0
5	6.850		0.0000	0.00000	0.00000	C8:0
6	8.500		0.0000	0.00000	0.00000	C10:0
7	9.500		0.0000	0.00000	0.00000	C11:0
8	10.611	BB	0.0258	6.33227	0.04763	C12:0
9	12.500		0.0000	0.00000	0.00000	C13:0
10	14.206	MM	0.0440	303.65549	2.28390	C14:0
11	15.000	BB	0.0438	3.12449	0.02350	C14:1
12	16.513	MM	0.0517	27.09106	0.20376	C15:0
13	17.900		0.0000	0.00000	0.00000	C15:1
14	19.201	MM	0.0743	1431.88989	10.76976	C16:0
15	19.815	MM	0.0631	330.03683	2.48233	C16:1
16	21.412	MM	0.0630	33.70829	0.25353	C16:2n4
17	21.933	MM	0.0679	29.71420	0.22349	C17:0
18	22.344	BV	0.0602	36.60550	0.27532	C16:3n4
19	22.647	MM	0.0737	9.60263	0.07222	C17:1
20	23.980	BB S	0.0622	62.43129	0.46957	C16:4n1
21	24.947	BB	0.0789	490.85535	3.69190	C18:0
22	25.572	MF	0.1306	4753.72266	35.75447	C18:1n9
23	25.682	FM	0.0572	346.51089	2.60623	C18:1n7
24	26.826	MM	0.0895	1793.14746	13.48691	C18:2n6
25	27.354	MM	0.0760	13.30876	0.10010	C18:2n4
26	27.612	MM	0.0713	10.19311	0.07667	C18:3n6
27	28.283	MM	0.0797	9.30147	0.06996	C18:3n4
28	28.676	MM	0.0739	658.30402	4.95134	C18:3n3
29	29.540	BB S	0.0645	95.34792	0.71715	C18:4n3
30	30.817	BB	0.0679	57.77829	0.43457	C20:0
31	31.197	MF	0.0732	52.26635	0.39311	C20:1n11
32	31.335	FM	0.0745	154.57469	1.16261	C20:1n9
33	32.696	BB	0.0751	21.02078	0.15810	C20:2n6
34	33.459	VB R	0.0757	8.18746	0.06158	C20:3n6
35	33.700		0.0000	0.00000	0.00000	C21:0
36	34.087	BV	0.0616	41.10044	0.30913	C20:4n6
37	34.600	VV	0.0711	7.20223	0.05417	C20:3n3
38	35.365	BB	0.0748	34.00395	0.25576	C20:4n3
39	36.020	VV R	0.0709	463.40442	3.48543	C20:5n3
40	36.635	BV	0.0707	37.06720	0.27880	C22:0
41	36.993	BV	0.0699	95.41463	0.71765	?

Sample Name: VIT25-7118

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
42	37.163	VB	0.0793	24.54923	0.18464	C22:1n9
43	38.900		0.0000	0.00000	0.00000	C22:2n6
44	39.068	BV	0.0711	20.75363	0.15610	C21:5n3
45	39.575	BV	0.0864	1267.28320	9.53170	C23:0
46	40.850	BV	0.0795	15.89827	0.11958	?
47	42.140	BV	0.0781	78.64299	0.59150	C22:5n3
48	42.719	BV	0.0843	23.31581	0.17537	C24:0
49	43.202	BV	0.0926	410.07080	3.08429	C22:6n3
50	43.477	VH	0.0875	38.04475	0.28615	C24:1n9

Totals : 1.32955e4

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

*** End of Report ***