


Sample Name: VIT25-7248

```
=====
Acq. Operator   :                               Seq. Line :    4
Acq. Instrument : GC7890B                       Location  :    4
Injection Date  : 7/15/2025 17:44:55             Inj       :    1
                                                Inj Volume : 1 µl
Acq. Method     : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M
Last changed    : 7/15/2025 14:51:21
Analysis Method : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M (Sequence Method)
Last changed    : 7/16/2025 9:08:32
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

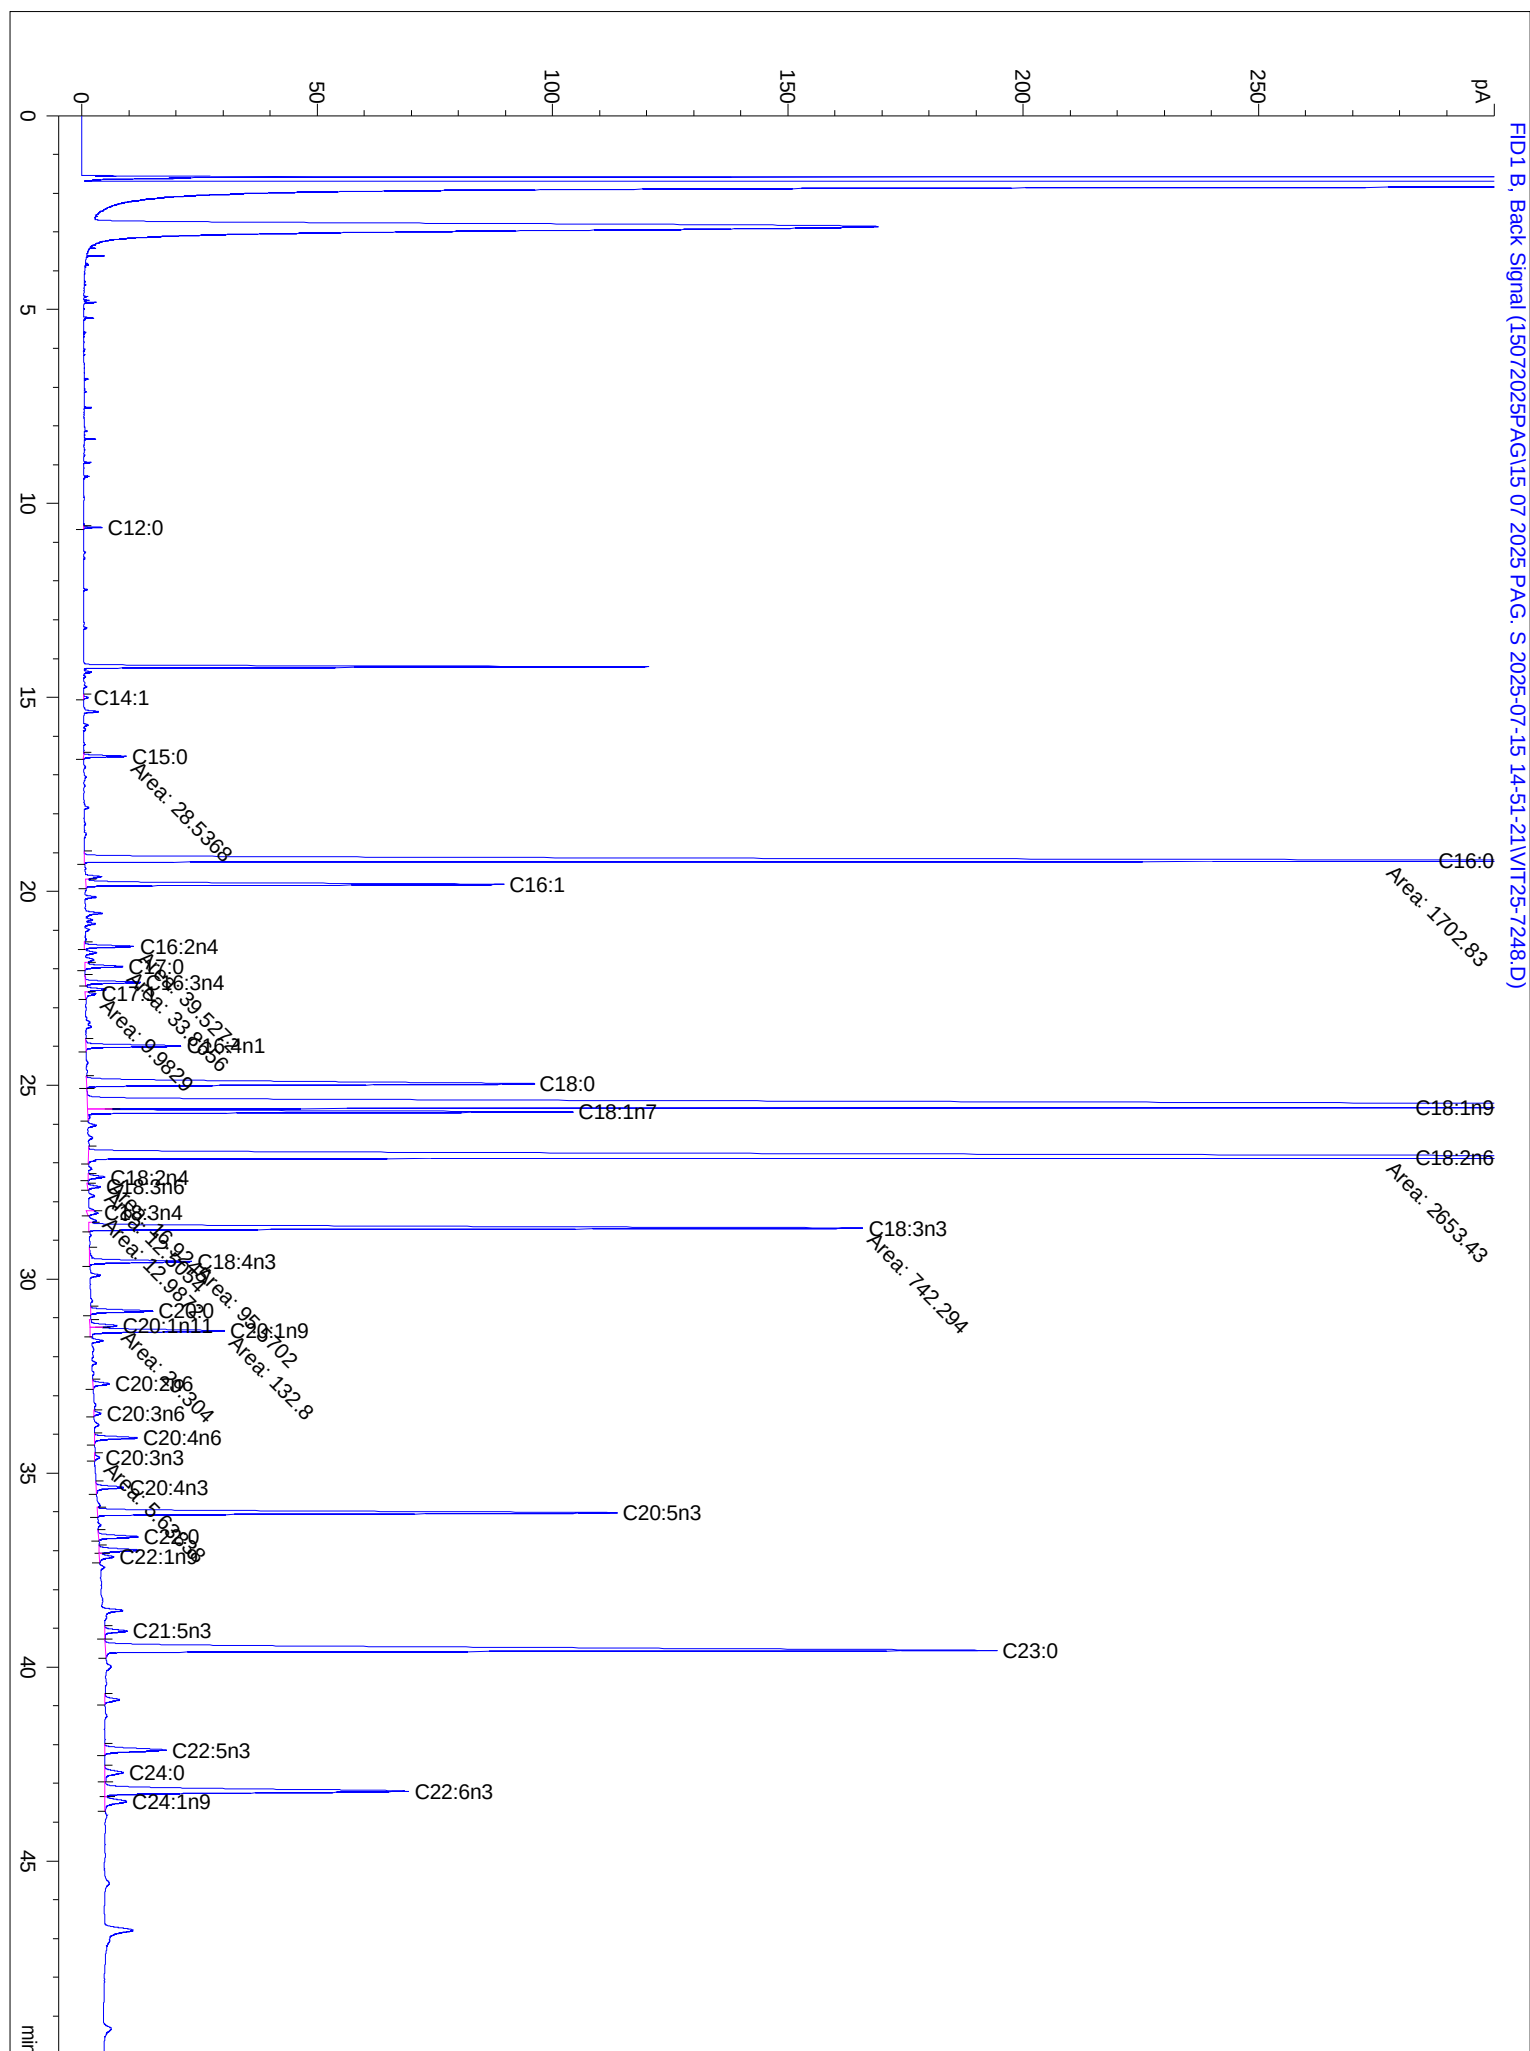

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 7/16/2025 9:08:31
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	0.000		0.0000	0.00000	0.00000	C18:2n6t
2	0.000		0.0000	0.00000	0.00000	C18:1n9t
3	3.450		0.0000	0.00000	0.00000	C4:0
4	5.255		0.0000	0.00000	0.00000	C6:0
5	6.850		0.0000	0.00000	0.00000	C8:0
6	8.500		0.0000	0.00000	0.00000	C10:0
7	9.500		0.0000	0.00000	0.00000	C11:0
8	10.610	BB	0.0261	6.63800	0.04636	C12:0
9	12.500		0.0000	0.00000	0.00000	C13:0
10	14.250		0.0000	0.00000	0.00000	C14:0
11	14.998	BB	0.0459	2.69563	0.01883	C14:1
12	16.509	MM	0.0518	28.53682	0.19932	C15:0
13	17.900		0.0000	0.00000	0.00000	C15:1
14	19.208	MM	0.0804	1702.83411	11.89356	C16:0
15	19.813	VB S	0.0566	331.85468	2.31786	C16:1
16	21.410	MM	0.0627	39.52722	0.27608	C16:2n4
17	21.929	MM	0.0696	33.86564	0.23654	C17:0
18	22.337	BV	0.0622	46.14004	0.32227	C16:3n4
19	22.646	MM	0.0756	9.98290	0.06973	C17:1
20	23.980	BB S	0.0626	83.24365	0.58142	C16:4n1
21	24.953	BB	0.0862	572.20990	3.99664	C18:0
22	25.569	BV	0.1012	4824.84326	33.69944	C18:1n9
23	25.679	VV R	0.0521	354.17770	2.47378	C18:1n7
24	26.854	MM	0.1004	2653.43433	18.53309	C18:2n6
25	27.359	MM	0.0769	16.92450	0.11821	C18:2n4
26	27.614	MM	0.0745	12.50540	0.08734	C18:3n6
27	28.289	MM	0.0905	12.98722	0.09071	C18:3n4
28	28.677	MM	0.0752	742.29419	5.18460	C18:3n3
29	29.537	MM	0.0734	95.57024	0.66752	C18:4n3
30	30.813	BB	0.0657	58.99881	0.41208	C20:0
31	31.190	MF	0.0855	29.30396	0.20468	C20:1n11
32	31.327	FM	0.0775	132.79994	0.92755	C20:1n9
33	32.691	BB	0.0740	17.83017	0.12454	C20:2n6
34	33.456	VV	0.0609	6.89922	0.04819	C20:3n6
35	33.700		0.0000	0.00000	0.00000	C21:0
36	34.086	BB	0.0670	43.56752	0.30430	C20:4n6
37	34.594	MM	0.0849	5.63838	0.03938	C20:3n3
38	35.362	BB	0.0771	29.52872	0.20625	C20:4n3
39	36.016	VB	0.0682	517.55127	3.61487	C20:5n3
40	36.632	BV	0.0694	41.36441	0.28891	C22:0
41	36.979	BV	0.0748	44.56679	0.31128	?

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
42	37.154	VB	0.0724	17.20849	0.12019	C22:1n9
43	38.900		0.0000	0.00000	0.00000	C22:2n6
44	39.071	BV	0.0646	23.82513	0.16641	C21:5n3
45	39.565	BB	0.0813	1180.41040	8.24466	C23:0
46	40.837	BV	0.0753	17.18727	0.12005	?
47	42.132	BV	0.0868	78.70470	0.54972	C22:5n3
48	42.715	BV	0.0904	28.51556	0.19917	C24:0
49	43.196	VV	0.0837	435.89856	3.04456	C22:6n3
50	43.460	VH	0.0986	37.21344	0.25992	C24:1n9

Totals : 1.43173e4

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====
*** End of Report ***