


```
=====
Acq. Operator   :                               Seq. Line :    6
Acq. Instrument : GC7890B                       Location  :    6
Injection Date  : 7/15/2025 19:38:49              Inj       :    1
                                                Inj Volume : 1 µl
Acq. Method     : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M
Last changed    : 7/15/2025 14:51:21
Analysis Method : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M (Sequence Method)
Last changed    : 7/16/2025 9:08:32
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

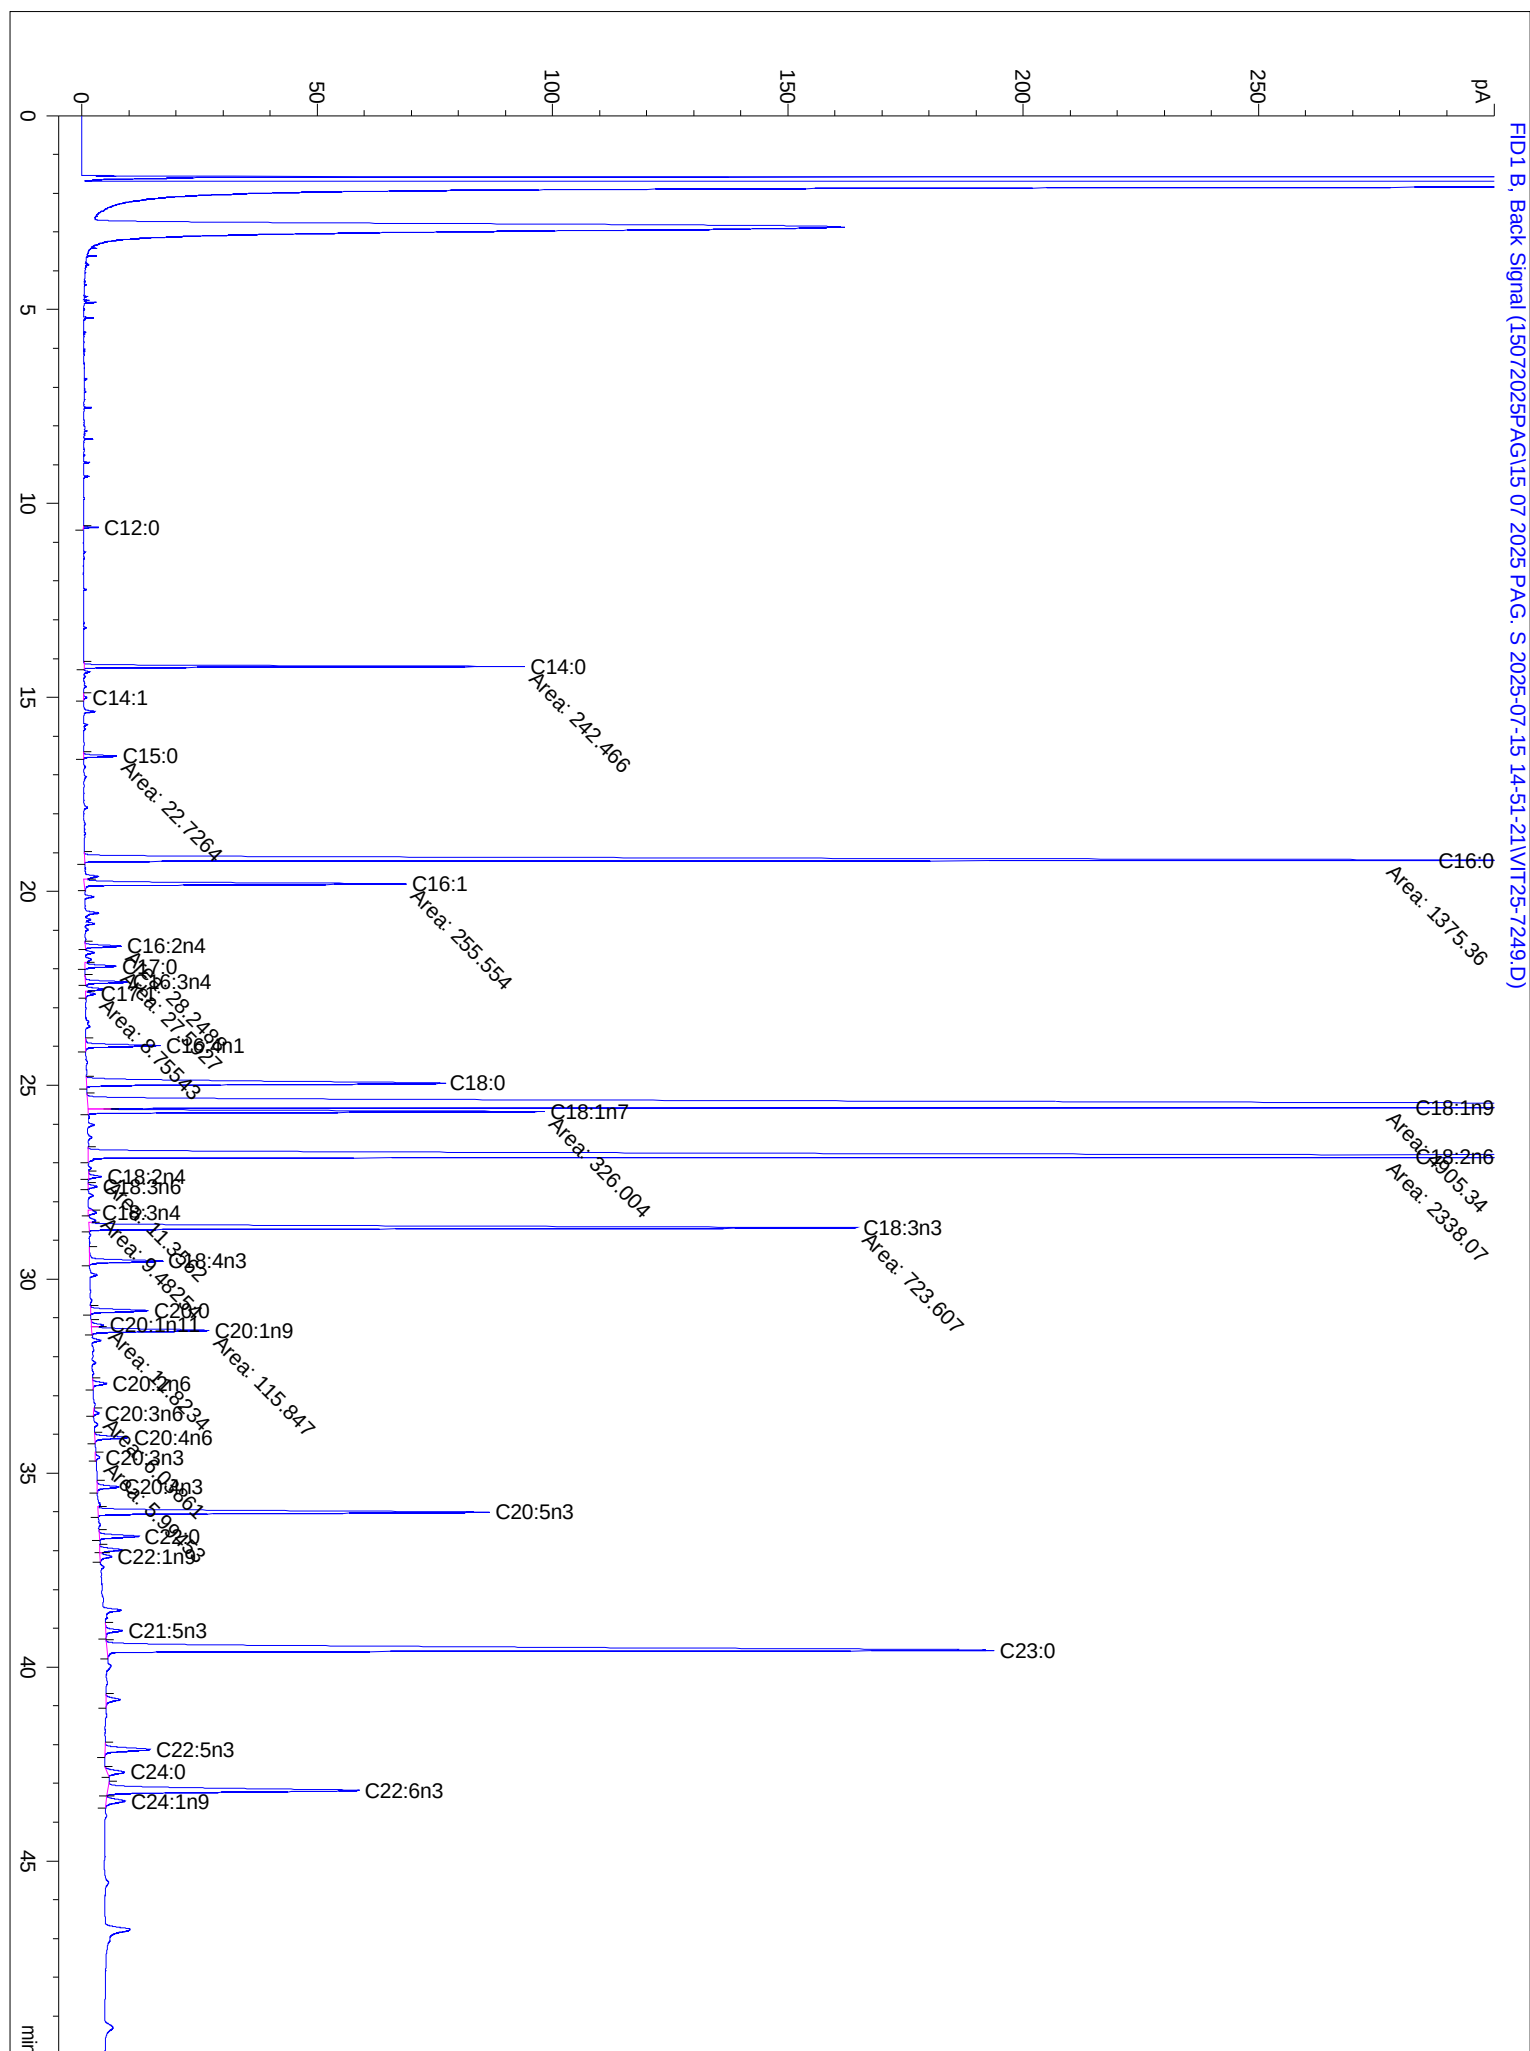

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 7/16/2025 9:08:31
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	0.000		0.0000	0.00000	0.00000	C18:2n6t
2	0.000		0.0000	0.00000	0.00000	C18:1n9t
3	3.450		0.0000	0.00000	0.00000	C4:0
4	5.255		0.0000	0.00000	0.00000	C6:0
5	6.850		0.0000	0.00000	0.00000	C8:0
6	8.500		0.0000	0.00000	0.00000	C10:0
7	9.500		0.0000	0.00000	0.00000	C11:0
8	10.608	BB	0.0262	5.39884	0.04034	C12:0
9	12.500		0.0000	0.00000	0.00000	C13:0
10	14.198	MM	0.0431	242.46582	1.81164	C14:0
11	14.993	BB	0.0461	2.15057	0.01607	C14:1
12	16.505	MM	0.0533	22.72638	0.16981	C15:0
13	17.900		0.0000	0.00000	0.00000	C15:1
14	19.191	MM	0.0733	1375.35718	10.27632	C16:0
15	19.803	MM	0.0623	255.55414	1.90944	C16:1
16	21.405	MM	0.0615	28.24878	0.21107	C16:2n4
17	21.922	MM	0.0687	27.59267	0.20617	C17:0
18	22.332	BV	0.0581	34.89588	0.26073	C16:3n4
19	22.640	MM	0.0708	8.75543	0.06542	C17:1
20	23.970	BB S	0.0546	61.94018	0.46280	C16:4n1
21	24.941	BB	0.0837	457.50879	3.41839	C18:0
22	25.561	MF	0.1300	4905.33838	36.65145	C18:1n9
23	25.674	FM	0.0560	326.00394	2.43582	C18:1n7
24	26.838	MM	0.0966	2338.07495	17.46951	C18:2n6
25	27.349	MM	0.0696	11.35617	0.08485	C18:2n4
26	27.603	BB	0.0598	7.84952	0.05865	C18:3n6
27	28.282	MM	0.0880	9.48254	0.07085	C18:3n4
28	28.665	MM	0.0738	723.60663	5.40661	C18:3n3
29	29.527	BB S	0.0688	69.64493	0.52037	C18:4n3
30	30.805	BB	0.0700	56.34497	0.42100	C20:0
31	31.178	MF	0.0750	11.82345	0.08834	C20:1n11
32	31.319	FM	0.0773	115.84709	0.86558	C20:1n9
33	32.684	BB	0.0742	15.61533	0.11667	C20:2n6
34	33.446	MM	0.0821	6.03861	0.04512	C20:3n6
35	33.700		0.0000	0.00000	0.00000	C21:0
36	34.074	BV	0.0657	34.10674	0.25484	C20:4n6
37	34.587	MM	0.1038	5.99453	0.04479	C20:3n3
38	35.351	BV	0.0671	22.46081	0.16782	C20:4n3
39	36.002	VV	0.0622	382.94717	2.86128	C20:5n3
40	36.622	BB	0.0731	41.11627	0.30721	C22:0
41	36.971	BV	0.0744	23.92142	0.17873	?

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
42	37.143	VB	0.0739	14.44187	0.10791	C22:1n9
43	38.900		0.0000	0.00000	0.00000	C22:2n6
44	39.055	BV	0.0718	18.76076	0.14018	C21:5n3
45	39.564	BV	0.0848	1248.42090	9.32789	C23:0
46	40.832	BB	0.0828	18.29489	0.13669	?
47	42.117	BV	0.0812	59.05698	0.44126	C22:5n3
48	42.703	BV	0.0803	23.73298	0.17733	C24:0
49	43.173	BV	0.0789	343.07831	2.56339	C22:6n3
50	43.448	BB	0.0879	27.79408	0.20767	C24:1n9

Totals : 1.33837e4

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====
*** End of Report ***