


```
=====
Acq. Operator   :                               Seq. Line :    8
Acq. Instrument : GC7890B                       Location  :    8
Injection Date  : 7/15/2025 21:32:31             Inj       :    1
                                                Inj Volume : 1 µl
Acq. Method     : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M
Last changed    : 7/15/2025 14:51:21
Analysis Method : C:\Chem32\1\Data\15072025PAG\15 07 2025 PAG. S 2025-07-15 14-51-21\CP-WAX
                  52 60m g100g.M (Sequence Method)
Last changed    : 7/16/2025 9:47:38
                  (modified after loading)
Additional Info : Peak(s) manually integrated
```

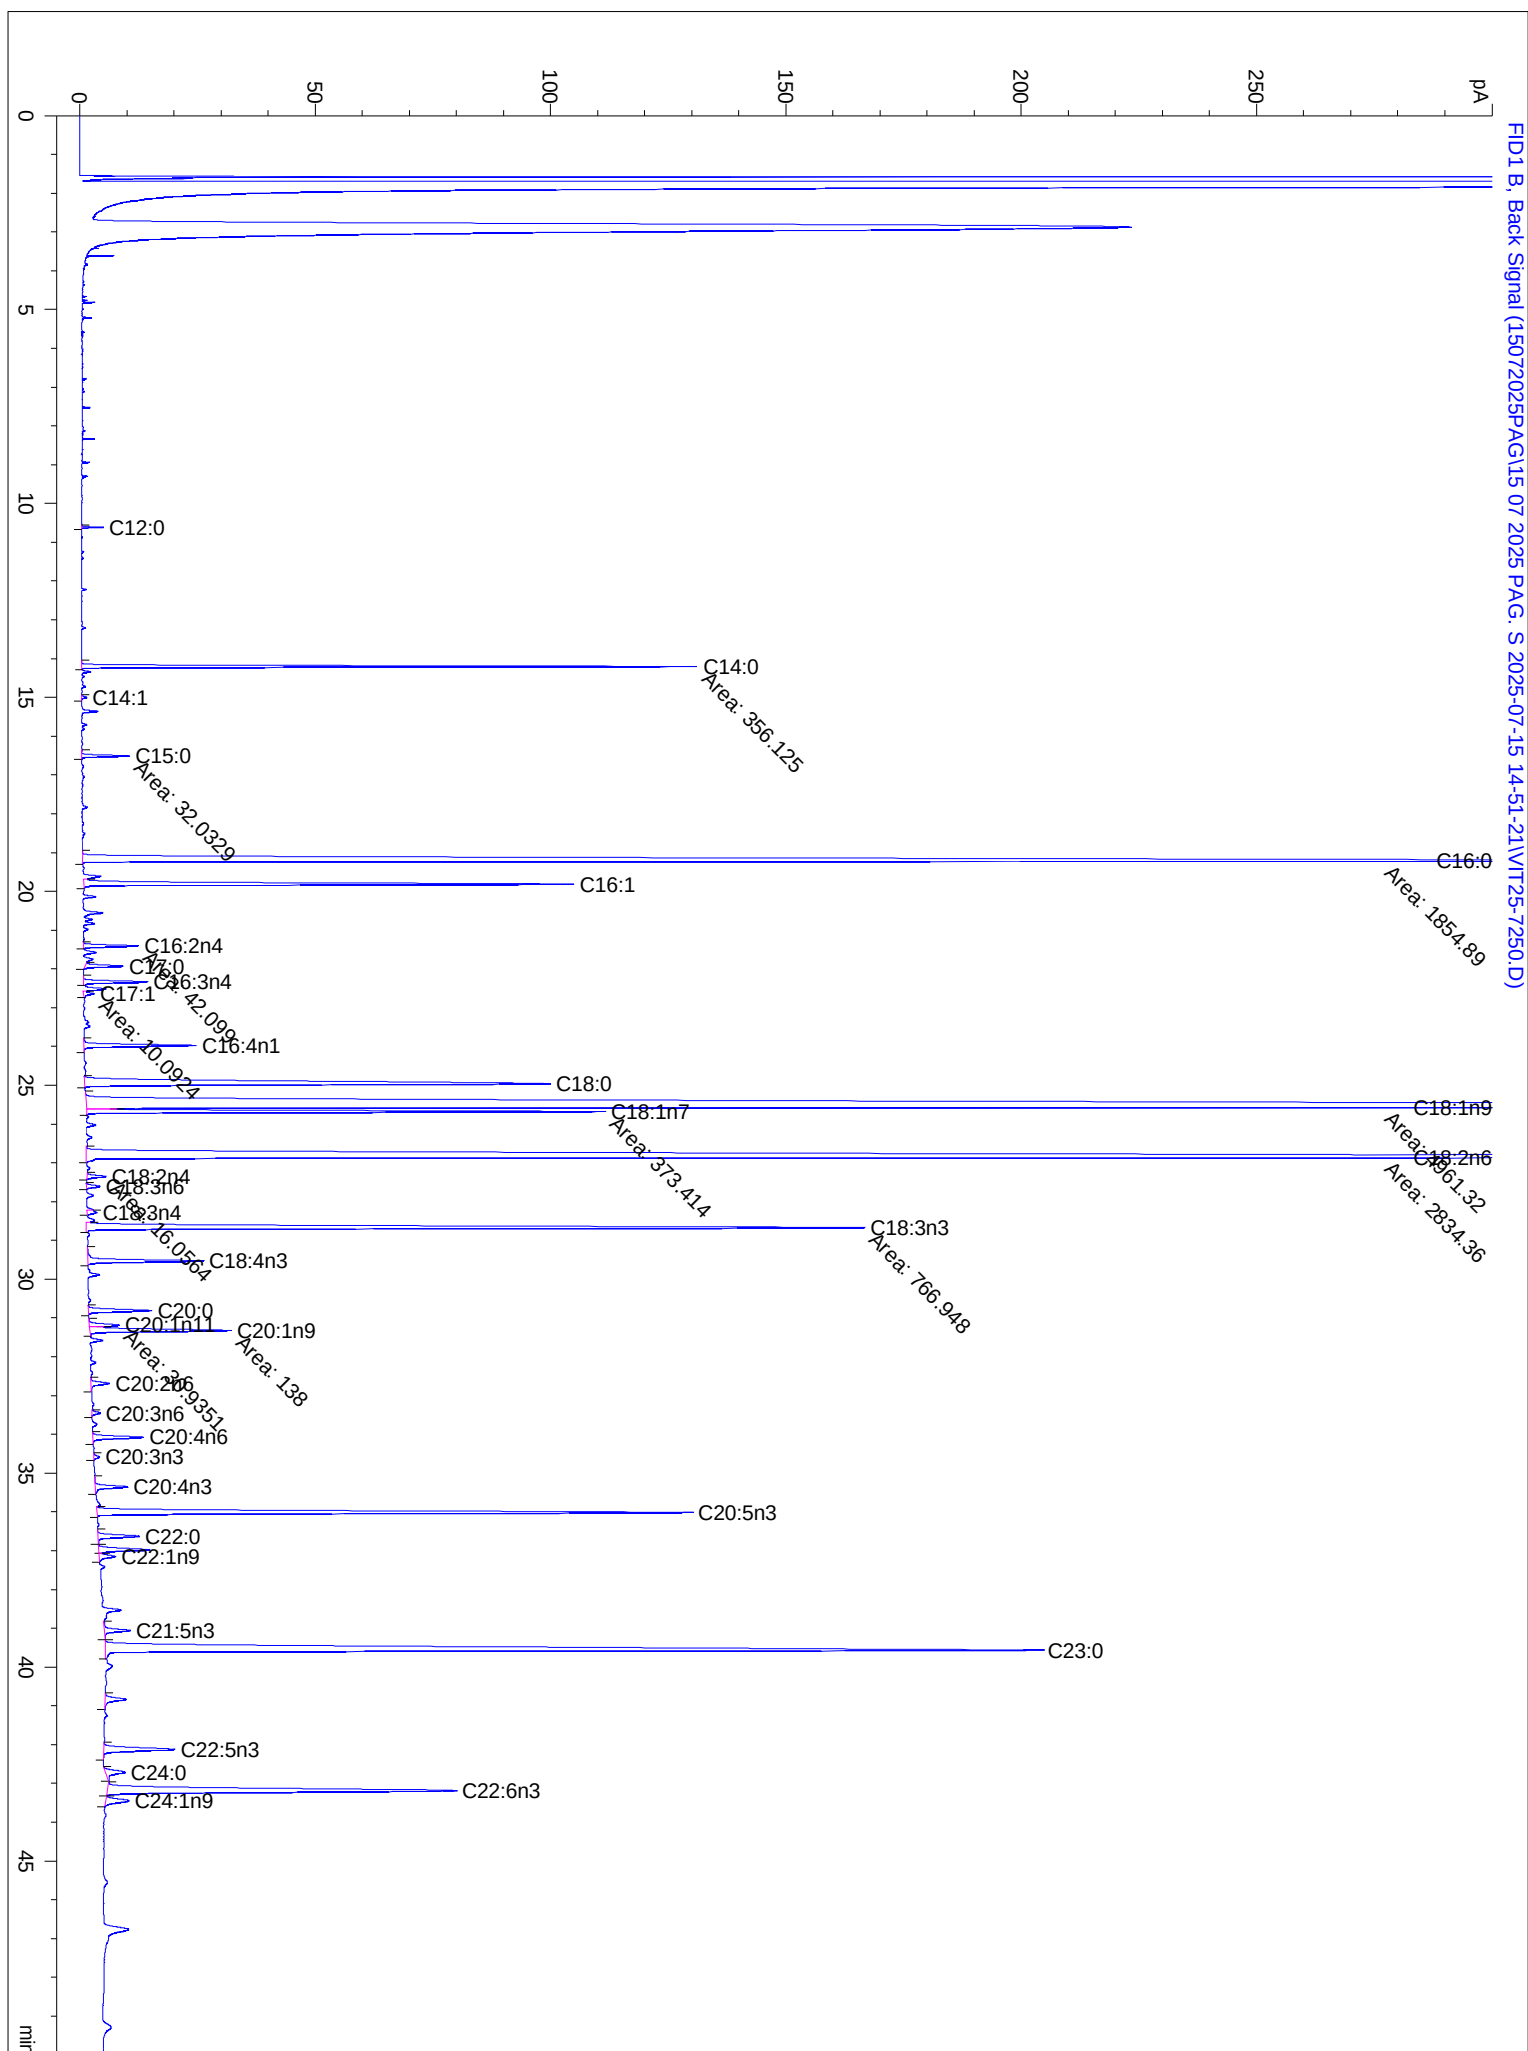

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 7/16/2025 9:47:37
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	0.000		0.0000	0.00000	0.00000	C18:2n6t
2	0.000		0.0000	0.00000	0.00000	C18:1n9t
3	3.450		0.0000	0.00000	0.00000	C4:0
4	5.255		0.0000	0.00000	0.00000	C6:0
5	6.850		0.0000	0.00000	0.00000	C8:0
6	8.500		0.0000	0.00000	0.00000	C10:0
7	9.500		0.0000	0.00000	0.00000	C11:0
8	10.606	BB	0.0265	7.69436	0.04930	C12:0
9	12.500		0.0000	0.00000	0.00000	C13:0
10	14.199	MM	0.0453	356.12469	2.28184	C14:0
11	14.990	BB	0.0426	3.17357	0.02033	C14:1
12	16.503	MM	0.0525	32.03295	0.20525	C15:0
13	17.900		0.0000	0.00000	0.00000	C15:1
14	19.207	MM	0.0819	1854.89270	11.88509	C16:0
15	19.809	VB S	0.0572	381.22296	2.44266	C16:1
16	21.399	MM	0.0605	42.09898	0.26975	C16:2n4
17	21.922	BB	0.0594	31.38311	0.20108	C17:0
18	22.327	BV	0.0625	53.02686	0.33977	C16:3n4
19	22.633	MM	0.0728	10.09242	0.06467	C17:1
20	23.969	BB S	0.0581	94.41179	0.60494	C16:4n1
21	24.954	BB	0.0827	607.87225	3.89490	C18:0
22	25.566	MF	0.1342	4961.31592	31.78926	C18:1n9
23	25.672	FM	0.0564	373.41425	2.39262	C18:1n7
24	26.847	MM	0.1016	2834.35522	18.16092	C18:2n6
25	27.344	MM	0.0678	16.05635	0.10288	C18:2n4
26	27.601	BB	0.0620	12.08181	0.07741	C18:3n6
27	28.274	VB	0.0573	9.43442	0.06045	C18:3n4
28	28.665	MM	0.0773	766.94788	4.91416	C18:3n3
29	29.524	BB S	0.0664	108.25174	0.69361	C18:4n3
30	30.803	BB	0.0666	61.17500	0.39197	C20:0
31	31.181	MF	0.0801	30.93509	0.19821	C20:1n11
32	31.314	FM	0.0764	137.99979	0.88422	C20:1n9
33	32.682	BV	0.0714	20.25531	0.12978	C20:2n6
34	33.444	VB	0.0615	8.38644	0.05374	C20:3n6
35	33.700		0.0000	0.00000	0.00000	C21:0
36	34.070	BB	0.0708	51.09999	0.32742	C20:4n6
37	34.579	BV	0.0638	5.70701	0.03657	C20:3n3
38	35.345	BB	0.0781	35.02002	0.22439	C20:4n3
39	36.006	VB	0.0657	593.66309	3.80385	C20:5n3
40	36.627	BB	0.0649	45.36720	0.29069	C22:0
41	36.970	BV	0.0700	54.43411	0.34878	?

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
42	37.144	VB	0.0717	19.37625	0.12415	C22:1n9
43	38.900		0.0000	0.00000	0.00000	C22:2n6
44	39.052	VV	0.0703	31.00910	0.19869	C21:5n3
45	39.555	BV	0.0862	1274.77966	8.16806	C23:0
46	40.826	BV	0.0794	27.02621	0.17317	?
47	42.116	BB	0.0738	91.51778	0.58639	C22:5n3
48	42.707	BB	0.0942	29.90694	0.19163	C24:0
49	43.182	BB	0.0929	498.49231	3.19405	C22:6n3
50	43.438	VH	0.0943	34.85627	0.22334	C24:1n9

Totals : 1.56069e4

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====
*** End of Report ***