




Certificate of Hydrophone Calibration

Hydrophone:	Onda HGL-1000 S/N: 1745
Cable/Adaptor:	NONE
External Amplifier:	NONE
Electrical Loading:	OpenCircuit
Temperature:	23.5 deg C
Calibration Completed:	22-Jun-2018
Data File Name:	HGL1000-1745_XXXXXX-XXXX-XX_XX_20180622.txt

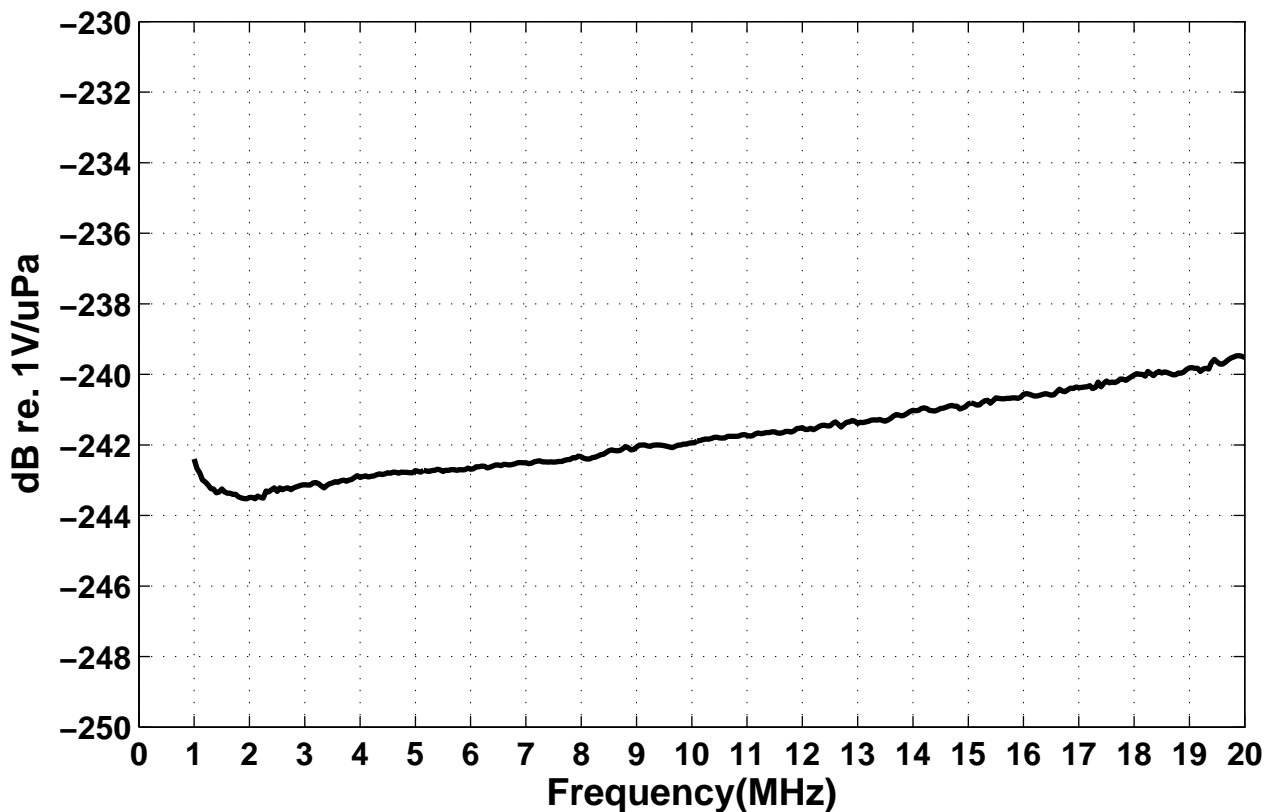

Calibration Method: Stepped single frequency comparison to Reference Standard

Measurement Uncertainty: 1-15 MHz: 1 dB; 15-20 MHz: 1.5 dB

Signature:  Date: 22-Jun-2018

1290 Hammerwood Avenue, Sunnyvale, CA 94089 T: (408) 745-0383 F: (408) 745-0956
www.ondacorp.com