




Certificate of Hydrophone Calibration

Hydrophone:	Onda HGL-0200 S/N: 1782
Cable/Adaptor:	NONE
External Amplifier:	Onda AG2010 S/N: 1199 (Nom. Gain: 20 dB)
Electrical Loading:	50Ohms
Temperature:	23.5 deg C
Calibration Completed:	29-Jan-2019
Data File Name:	HGL0200-1782_AG2010-1199-20_xx_20190129.txt

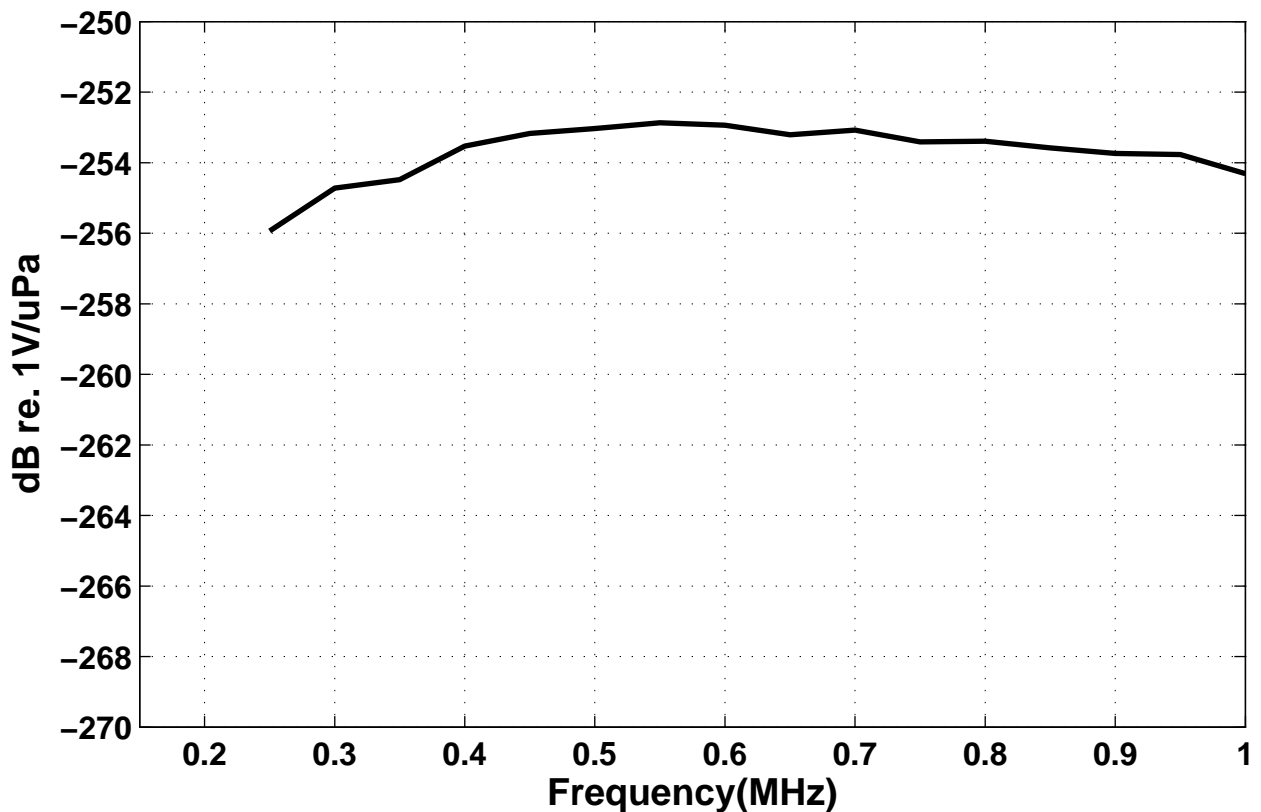

Calibration Method: Stepped single frequency comparison to Reference Standard

Measurement Uncertainty: 0.25-0.5 MHz: 3.0 dB; 0.5-1 MHz: 1.5 dB

Signature:

A handwritten signature in blue ink, appearing to be "J. Lee".

Date: 29-Jan-2019

1290 Hammerwood Avenue, Sunnyvale, CA 94089 T: (408) 745-0383 F: (408) 745-0956
www.ondacorp.com