



BESTLABS SINGAPORE

Bestlabs Singapore Pte. Ltd. | Company Registration no. 201728718W

19 Senoko Loop, Level 3, Singapore 758169

+65 6914 7777



+65 9859 7777 / +65 9850 7777



sales@calibration.sg



www.calibration.sg

CERTIFICATE
CALIBRATION
SERVICE

CERTIFICATE NO. : BLE2605250-2

PAGE 1 OF 3

SUBMITTED TO :

Kenyon Pte Ltd
8 Loyang Crescent
Singapore 509016

REFERENCE NO. : BSO-26-005250

RECEIVED DATE : 04-Jun-2026

ISSUED DATE : 05-Jun-2026



Bestlabs organization and practices have been compliance to the quality requirements of ISO 17025 in accordance with the principles of ISO 9001.

The reference measurement standards used are traceable to the International System of Units (SI) through National Metrology Centre, (NMC,SINGAPORE) and/or other National Standards.

INSTRUMENT		INSULATION TESTER			
MANUFACTURER	MEGGER	AMB. TEMPERATURE	(21 ± 2) °C		
MODEL NO.	MIT310	RELATIVE HUMIDITY	(55 ± 10) % relative humidity		
SERIAL NO.	102109639	CALIBRATED DATE	05-Jun-2026		
RANGE	(MULTIRANGE) .	DUE DATE	04-Jun-2027		
TAG NO.	ELECT-102109639	-	-		
PART NO.	-	-	-		
LOCATION	-	-	-		
CALIBRATION AT	BLS Laboratory	-	-		
MEASUREMENT TRACEABILITY					
REFERENCE STANDARDS	CERTIFICATE NO.	SERIAL NO.	TAG NO.	CAL. DATE	DUE DATE
MULTIFUNCTION ELECTRICAL TESTER CALIBRATOR	0104652	518930716	BS 1520	13-Sep-2025	12-Sep-2026
MULTIFUNCTION CALIBRATOR	1500428677/1500428630	2424603	BS 1697	15-May-2026	14-May-2027
METHOD OF CALIBRATION: FSE 02 , FSE 03 , FSE 04 & FSE 05					

NOTES:

- The results of the calibration are given on the attached following pages.
- The expanded uncertainty of measurement associated with the calibration is estimated at a confidence level of approximately 95%.
- No adjustment was done unless otherwise stated.
- The user should determine the suitability of the instrument for its intended use.
- The reports shall not be reproduced except in full, without written approval by management representative of BESTLABS SINGAPORE PTE LTD.
- Only DC Voltage, AC Voltage @ 50Hz, Resistance test and Insulation test function was calibrated.

N MANOHARAN
CALIBRATION OFFICER

DURAI SIVA
APPROVING OFFICER

YOUR BEST ALLIANCE



BESTLABS SINGAPORE

Bestlabs Singapore Pte. Ltd. | Company Registration no. 201728718W

📍 19 Senoko Loop, Level 3, Singapore 758169

☎ +65 6914 7777



+65 9859 7777 / +65 9850 7777



sales@calibration.sg



www.calibration.sg

CERTIFICATE
CALIBRATION
SERVICE

CERTIFICATE NO. : BLE2605250-2

PAGE 2 OF 3

TEST RESULTS :

REFERENCE READING	LOW LIMIT	MEASURED READING	HIGH LIMIT	EXPANDED UNCERTAINTY	COVERAGE FACTOR
DC VOLTAGE TEST					(k)
100 Vdc	97	100	103	0.58 Vdc	2.00
200 Vdc	196	200	204	0.58 Vdc	2.00
300 Vdc	295	300	305	0.58 Vdc	2.00
400 Vdc	394	399	406	0.58 Vdc	2.00
500 Vdc	493	499	507	0.58 Vdc	2.00
AC VOLTAGE TEST @50Hz					(k)
100 Vac	97	100	103	0.58 Vac	2.00
200 Vac	196	199	204	0.58 Vac	2.00
300 Vac	295	299	305	0.58 Vac	2.00
400 Vac	394	401	406	0.61 Vac	2.00
500 Vac	493	501	507	0.61 Vac	2.00
CONTINUITY TEST					(k)
1.00 Ω	0.95	1.02	1.05	0.038 Ω	2.00
10.0 Ω	9.5	10.2	10.5	0.23 Ω	2.00
30.0 Ω	28.9	30.2	31.1	0.23 Ω	2.00
50.0 Ω	48.3	50.3	51.7	0.23 Ω	2.00
90.0 Ω	87.1	90.3	92.9	0.23 Ω	2.00
INSULATION TEST 999 Mohm @ 250V RANGE:					(k)
100.0 M Ω	94.5	101.5	105.5	3 M Ω	2.00
500 M Ω	470	518	530	7.5 M Ω	2.00
900 M Ω	850	923	950	7.5 M Ω	2.00
INSULATION TEST 999 Mohm @ 500V RANGE:					(k)
100.0 M Ω	94.5	101.1	105.5	3 M Ω	2.00
500 M Ω	470	509	530	7.5 M Ω	2.00
900 M Ω	850	918	950	7.5 M Ω	2.00

YOUR BEST ALLIANCE





BESTLABS SINGAPORE

Bestlabs Singapore Pte. Ltd. | Company Registration no. 201728718W

19 Senoko Loop, Level 3, Singapore 758169

+65 6914 7777



+65 9859 7777 / +65 9850 7777



sales@calibration.sg



www.calibration.sg

CERTIFICATE
CALIBRATION
SERVICE


CERTIFICATE NO. : BLE2605250-2

PAGE 3 OF 3

TEST RESULTS :

REFERENCE READING	LOW LIMIT	MEASURED READING	HIGH LIMIT	EXPANDED UNCERTAINTY	COVERAGE FACTOR
INSULATION TEST 999 Mohm @ 1000V RANGE:					(k)
100.0 MΩ	94.5	100.9	105.5	3 MΩ	2.00
500 MΩ	470	507	530	7.5 MΩ	2.00
900 MΩ	850	911	950	7.5 MΩ	2.00

***** End Of Test Results *****

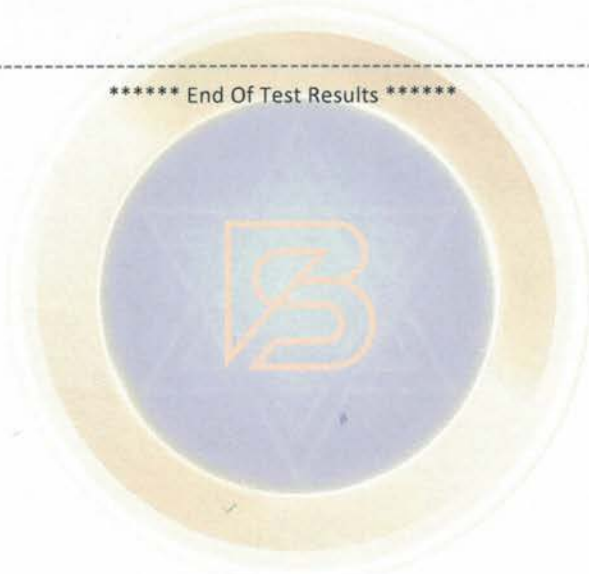

YOUR BEST ALLIANCE

