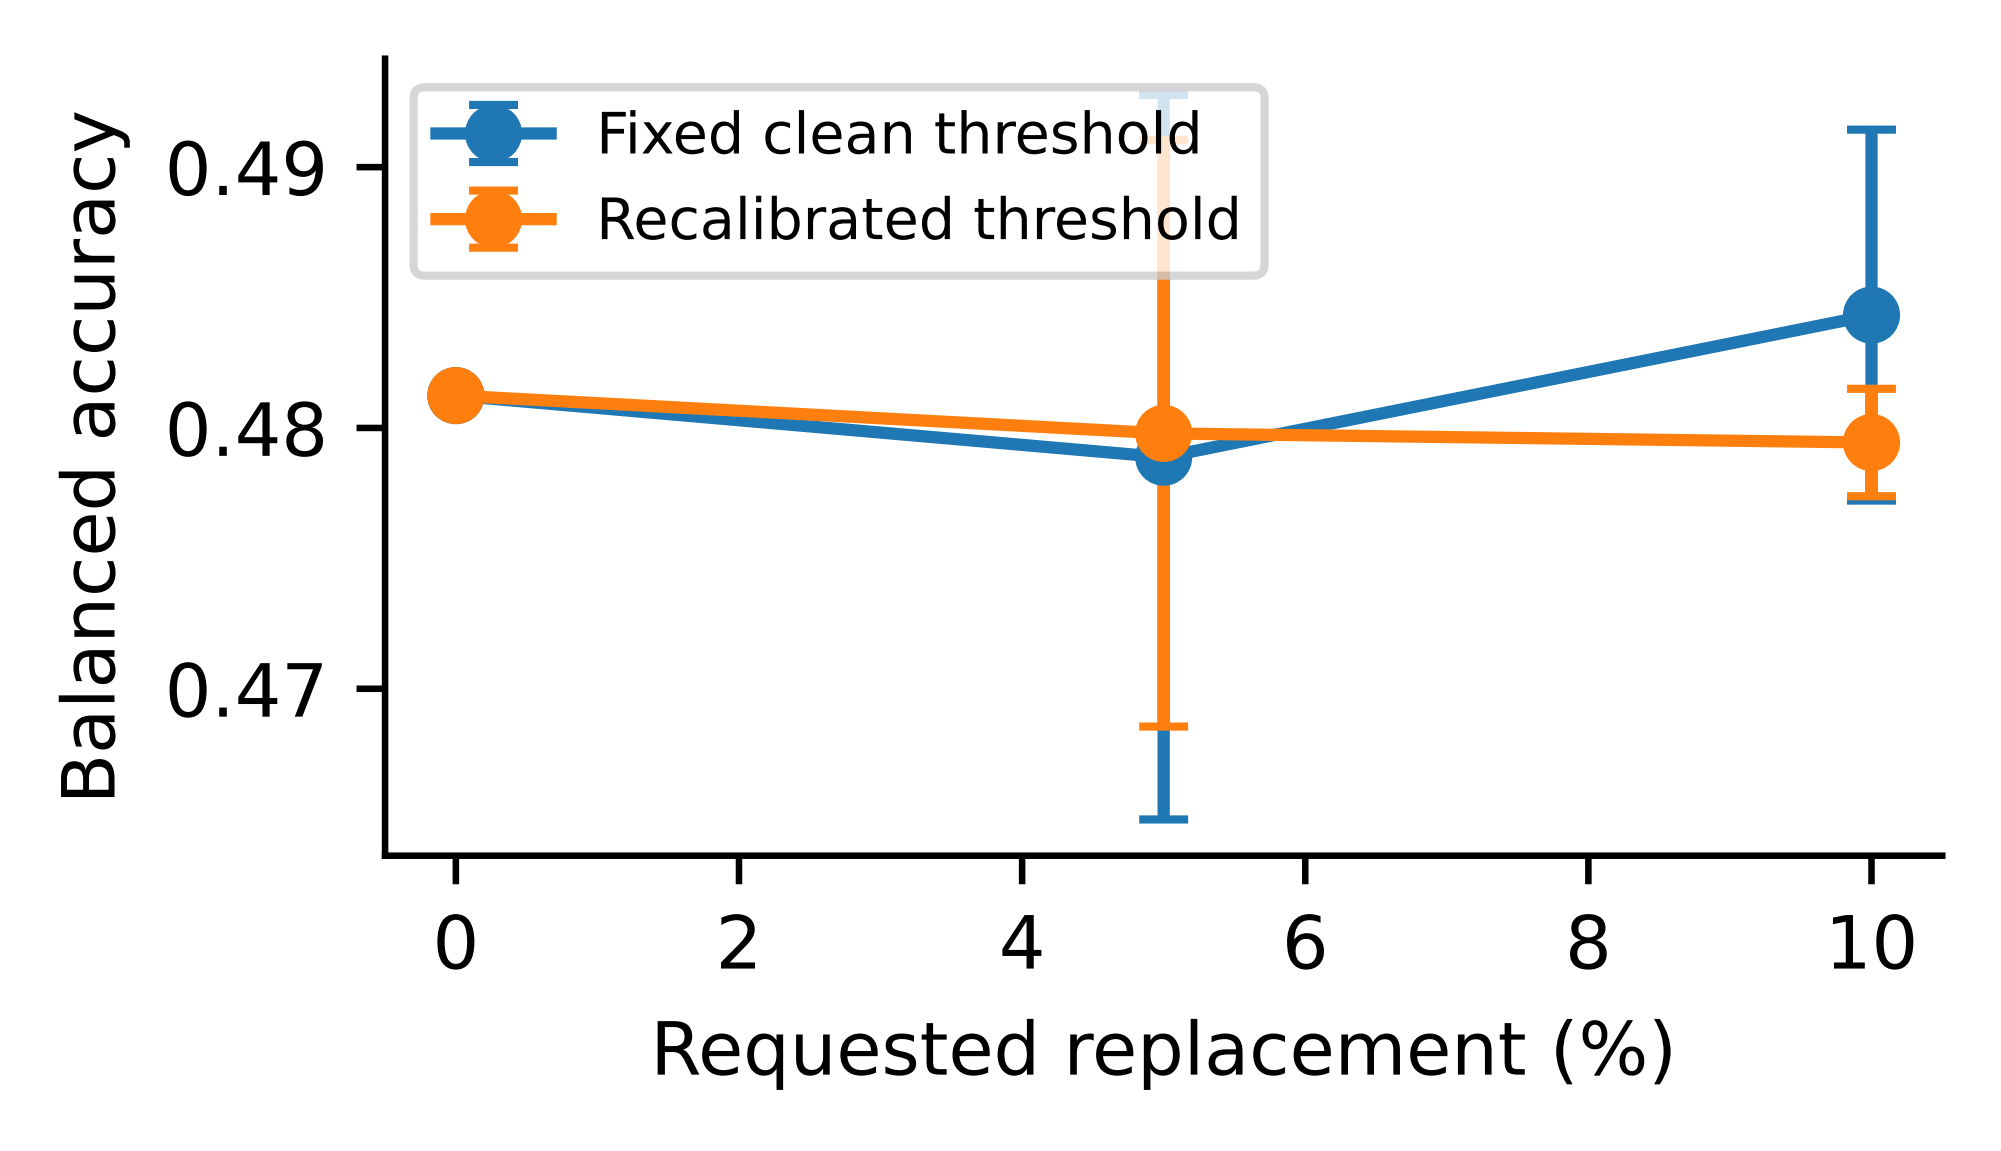
Fixed clean threshold
Recalibrated threshold
Balanced accuracy
0.49
0.48
0.47
0
2
4
6
8
10
Requested replacement (%)