BATCH REPORT

Lot L-2611-0390 · 24 ChArUco targets

CUSTOMER & ORDER

Customer	Example Automation AG
PO	PO-4500123456
Part number	CT-CHA-C-200150-6X6
Lot	L-2611-0390

BATCH

Quantity	24 boards
Serial range	000320–000343
Inspection period	2026-11-09–2026-11-13
Master board	S1b master board SN 000300

RELEASED BOARDS

PASS

All 23 released boards meet the stated limits. SN 000337 is rejected for flatness and not delivered.

24 inspected · 23 released · 1 rejected
Pitch ±2 µm · flatness ≤20 µm

1 Board summary

deviations in µm

SERIAL	PITCH X DEV (µm)	PITCH Y DEV (µm)	FLATNESS (µm)	RESULT
000320	−0.2	−1.0	10.8	PASS
000321	−0.7	+0.2	11.1	PASS
000322	+0.1	−0.6	12.0	PASS
000323	−0.5	−0.8	10.2	PASS
000324	−0.2	+0.2	9.6	PASS
000325	0.0	−0.9	12.2	PASS
000326	−0.3	+0.2	8.0	PASS
000327	−0.7	+0.2	9.8	PASS
000328	−0.6	+0.3	13.0	PASS
000329	+0.4	+0.4	12.4	PASS
000330	0.0	+0.2	15.1	PASS
000331	−1.1	0.0	9.9	PASS
000332	+0.9	−0.3	10.2	PASS
000333	+0.2	−0.1	10.6	PASS
000334	+0.1	−0.2	13.2	PASS
000335	−0.4	−0.3	10.2	PASS
000336	−0.1	+0.4	12.2	PASS
000337	+0.8	−1.5	23.0	☒ **FAIL**
000338	+0.5	+0.2	11.6	PASS
000339	+1.2	+1.4	10.1	PASS
000340	+0.4	+0.9	10.3	PASS
000341	+0.7	+0.2	12.3	PASS
000342	+1.1	−0.2	10.3	PASS
000343	+0.6	−0.5	10.8	PASS

LIMITS & METHOD

Pitch X and Pitch Y limits are ±2 µm. Flatness upper limit is 20 µm; values are measured at 25 points per board.

2 Batch statistics

all inspected boards


METRIC	N	MEAN (µm)	STD (µm)	MIN (µm)	MAX (µm)	CPK
Pitch X deviation	24	+0.1	0.59	−1.1	+1.2	1.09
Pitch Y deviation	24	−0.1	0.60	−1.5	+1.4	1.07
Flatness	24	+11.6	2.78	+8.0	+23.0	1.00

Cpk is calculated over all 24 inspected boards using population standard deviation. Pitch uses two-sided limits (±2 µm); flatness uses the upper limit only (≤20 µm).

SAMPLE

3 Pitch control chart

tolerance ±2 µm

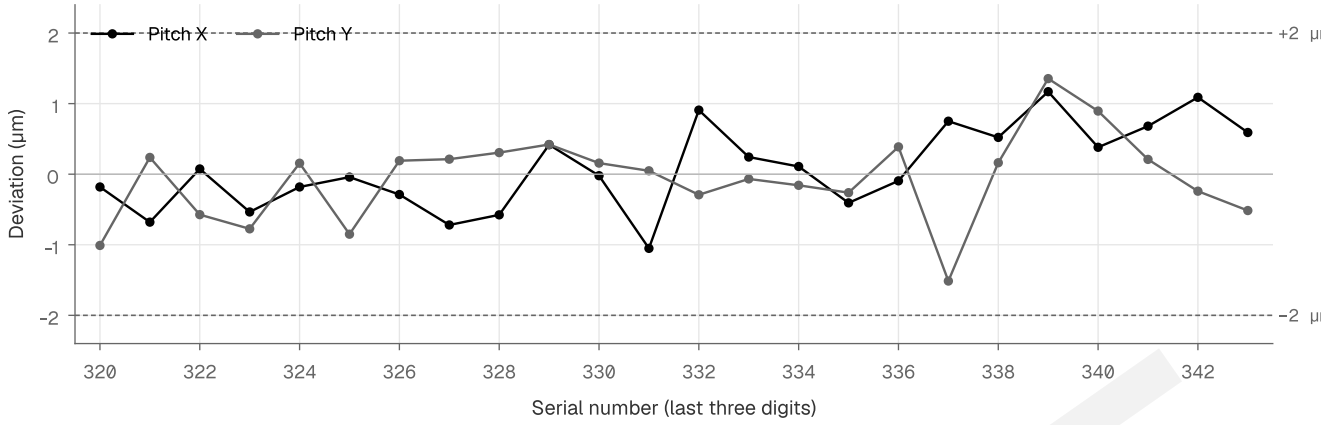

Pitch X shown in black; Pitch Y shown in grey. Dashed lines denote the two-sided pitch tolerance.

4 Master comparison

S1b · SN 000300

FEATURE	REFERENCE (µm)	BEFORE BATCH (µm)	AFTER BATCH (µm)	MAX DIFFERENCE (µm)	U (k=2) (µm)	RESULT
Pitch X deviation	0.0	+0.2	+0.3	0.3	1.5	PASS
Pitch Y deviation	0.0	−0.2	−0.1	0.2	1.5	PASS
Flatness	9.5	9.7	9.6	0.2	1.5	PASS

Measurements of S1b master board SN 000300 before and after the batch remain within U = 1.5 µm (k = 2) of the reference values.

5 Nonconforming board

REJECTED

000337 — flatness 23.0 µm; upper limit 20.0 µm. Board rejected.

6 Statement

The batch identified above was inspected against the stated pitch and flatness limits. Twenty-three boards met the applicable limits; SN 000337 was rejected for flatness above the upper limit.

This batch report is issued by the manufacturer and is not an accredited calibration certificate.

SIGNED

JG

JG · Inspector · 2026-11-14
Printed signature

CALIB.TOOLS
LOT L-2611-0390
INSPECTED
2026-11-14
JG
DIMENSIONAL INSPECTION

calib.tools/verify/L-2611-0390

SAMPLE