CALIBRATION QUALITY REPORT

Camera calibration diagnostic

FREE DIAGNOSTIC · camera solution and capture coverage

CALIBRATION GRADE

B

Conditioning requires additional coverage.
RMS 0.142 px · coverage 66.2 % · 2 views rejected before final solve.


28 / 30 used
2448 × 2048 px

RMS REPROJECTION	MAX PER-IMAGE	COVERED GRID	REJECTED
0.142 px	0.152 px	66.2 %	2 views


1 Input snapshot

Camera model	[User camera] 5 MP GigE, 2448 × 2048
Pixel pitch / lens	3.45 µm / 12 mm
Images supplied	30 · 28 used · 2 rejected
Target	CT-CHA-C-200150-6X6 · SN 000311
Target inspection data	CT-IR-000311 imported
Software	OpenCV 5.0.0 · calibrateCameraExtended

2 Diagnostic overview

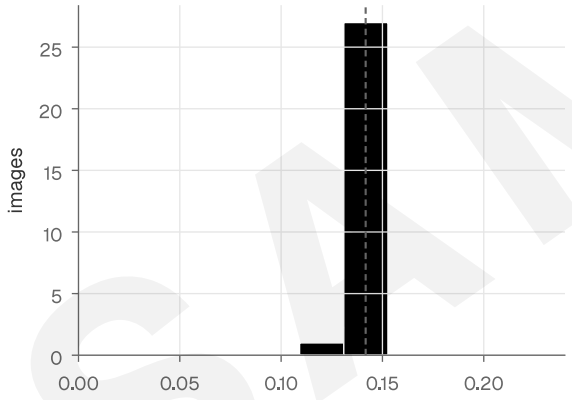

Histogram · retained per-image RMS. Dashed line: final RMS.

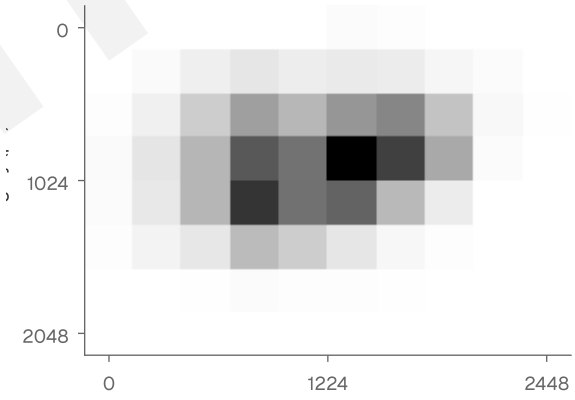

Coverage heatmap · 28 retained views; black = more detected corners.

3 Recommendations

- Recapture rejected views 09, 24 with focus locked; do not include them in the next solve.
- Add three captures with the target projected into the lower-right image region, at 0.45–0.80 m and 20–35° tilt.
- Retain the current centre/edge range and repeat the solve after the coverage grid exceeds 75 % for grade A.

GRADE RUBRIC A RMS ≤ 0.20 px, ≥ 75 % grid, ≤ 2 rejected · B RMS ≤ 0.30 px, ≥ 55 %, ≤ 3 · C RMS ≤ 0.50 px, ≥ 35 %, ≤ 5 · D otherwise. All three conditions apply within each grade.

STATEMENT

Computed from user-supplied data; Calib.Tools has not verified the images or the camera.

SAMPLE