Dexcom CLARITY

Clinically Relevant Insights in Minutes

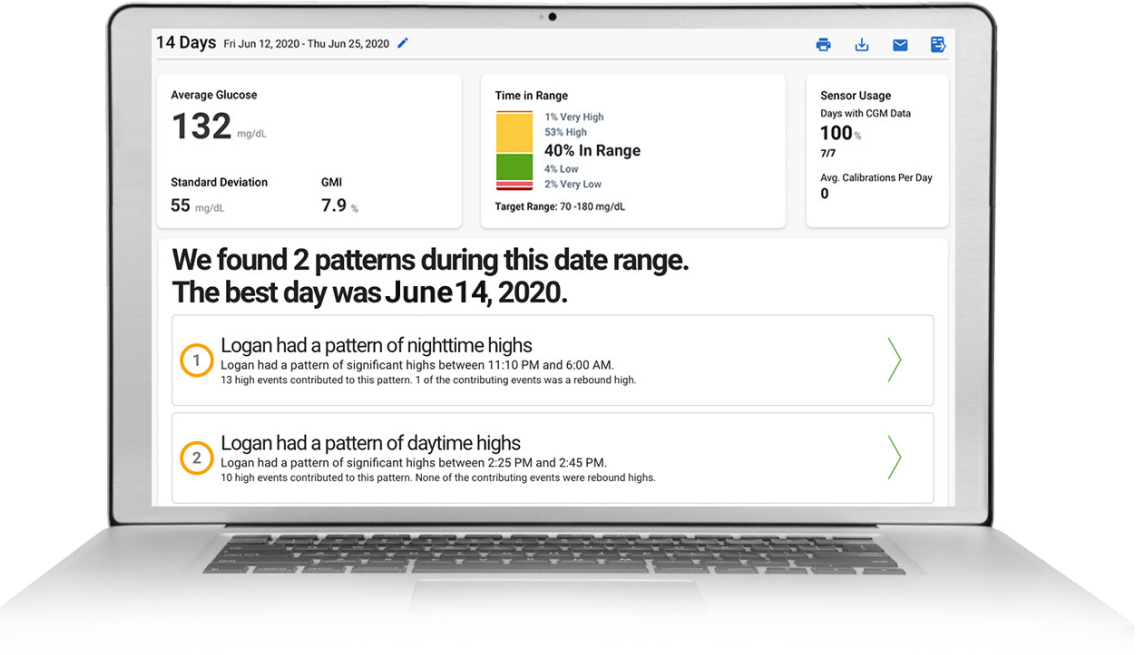

Avid Dexcom CLARITY users* spent 15% more time in range than non-users on average.[1]

*Avid users have 4 or more monthly log-ins to Dexcom CLARITY.

[1] Parker AS, et al. Diabetes Technol Ther. 2018;20(S1):A-27.

Dexcom CLARITY

Evaluate relevant glucose patterns and trends to help make diabetes management decisions from your clinic computer with Dexcom CLARITY.

With Dexcom CLARITY, you create patient accounts to upload and track continuous glucose monitoring (CGM) data during visits. View interactive reports, then save and print as needed. Invite patients to use Dexcom CLARITY and share their CGM data with your clinic for more efficient appointments.

Register your clinic for free at clarity.dexcom.com/professional

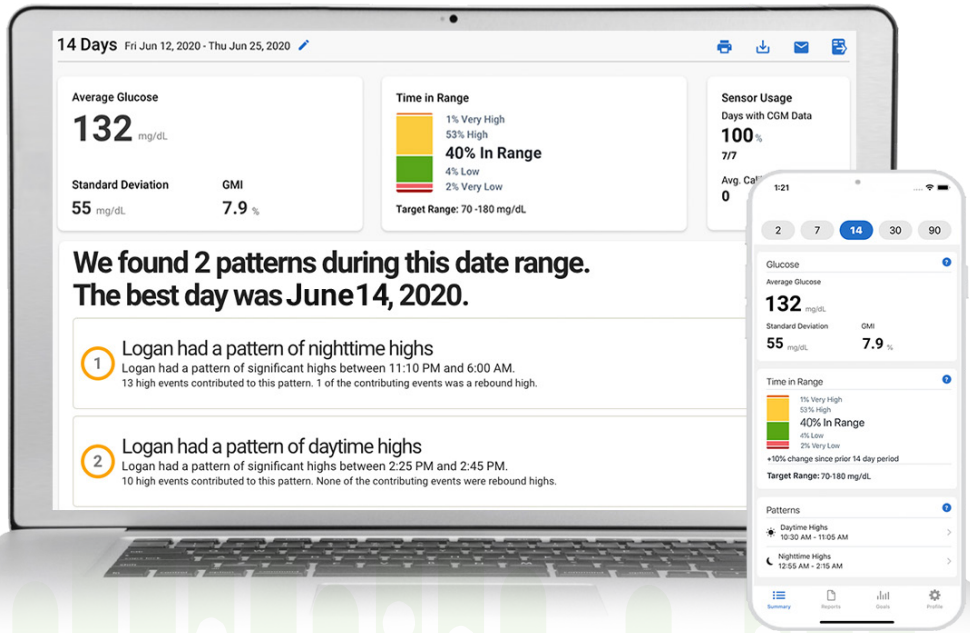

Intended Use/Safety Statement

The web-based Dexcom CLARITY software is intended for use by both home users and healthcare professionals to assist people with diabetes and their healthcare professionals in the review, analysis, and evaluation of CGM data to support effective diabetes management. WARNING: Treatment decisions, like treating for a low or dosing for a high, should not be made based on this software. Home users should follow instructions on the CGM system. WARNING: The software is not intended to replace self-monitoring practices as advised by a healthcare professional. CAUTION: Dexcom CLARITY provides recently available CGM information from the Dexcom CGM app or receiver. Since the smartphone system sends data to the Dexcom server, the information is always older than the real-time data displayed on the user's CGM app or receiver. Use the current information on the CGM app or receiver for treatment decisions, not the information from Dexcom CLARITY as that information is outdated. CAUTION: The software does not provide any medical advice and should not be used for that purpose. Home users must consult a healthcare professional before making any medical interpretation and therapy adjustments from the information in the software. CAUTION: Healthcare professionals should use information in the software in conjunction with other clinical information available to them. CAUTION: Federal (US) law restricts this device to sale by or on the order of a licensed healthcare professional.

©2017-2020 Dexcom and Dexcom CLARITY are registered trademarks of Dexcom, Inc. in the United States and may be in other countries. LBL013741 Rev010 MT23647

Overview Report

The Overview report presents a summary of the most relevant clinical patterns. This quick summary can help focus the discussion on areas contributing to hyper- and hypoglycemia. This report summarizes the quality of glucose control via metrics and identifies daytime and nighttime patterns of highs and lows for the date range selected.

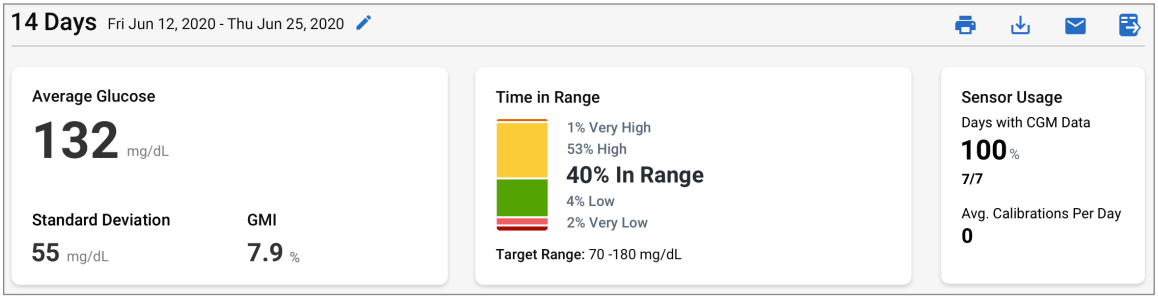

Average Glucose is the average of all the CGM glucose readings from the selected date range. Knowing the average glucose gives you a good place to start when trying to get numbers into target.

Standard Deviation reflects how much CGM glucose readings rise and fall also known as glycemic variability.

GMI (Glucose Management Indicator) approximates the laboratory A1C level expected based on average glucose measured using CGM values derived from at least 12 days of CGM data.

Time in Range The percentage of time that glucose levels are in low, target, and high ranges. The following are recommended ranges from an international consensus. Dexcom CLARITY ranges may be different than Dexcom CGM alerts. Changes made here apply only to Dexcom CLARITY.

- Target Range: 70-180 mg/dL
- Very High: Above 250 mg/dL
- Very Low: Below 54 mg/dL

Sensor Usage shows the number of days during the reporting period with at least 50% CGM readings and the daily average calibrations you enter. Only days with at least 50% CGM readings are included. The Dexcom G6 system is approved for use without calibrations.

Patterns Report

With Patterns, dive deeper with a daily micro view of patient control. Identified patterns begin discussions of what, why, and how to address issues and opens the door to patient education in managing their diabetes. If patients enter events into their CGM receiver, such as exercise, an icon displays below the graph to help pinpoint contributing factors. Significant data contributing to the pattern are shown in white sections.

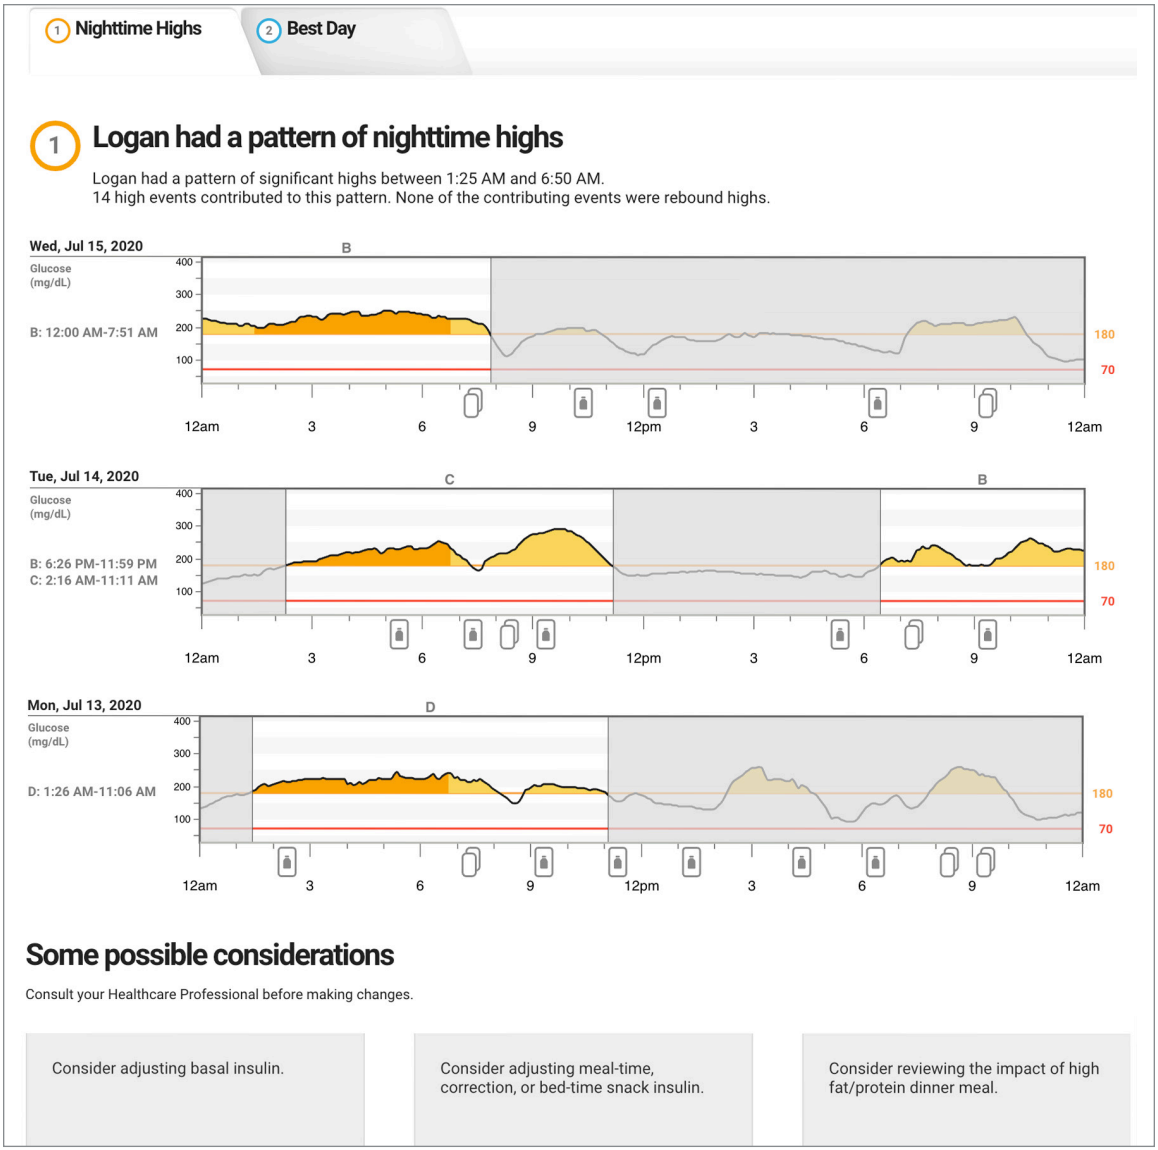

Trends Report

Trends is a holistic visual representation of patterns. It helps prioritize clinical issues based on discussions with the patient. In this report:

- Longer bars represent greater glycemic variability.
- Clinically significant hypoglycemia patterns are red - the most significant are bright red.
- Hyperglycemia patterns are yellow - the most significant are bright yellow.
- Outlier data is removed to help focus on patterns, the top 25% and bottom 15%.

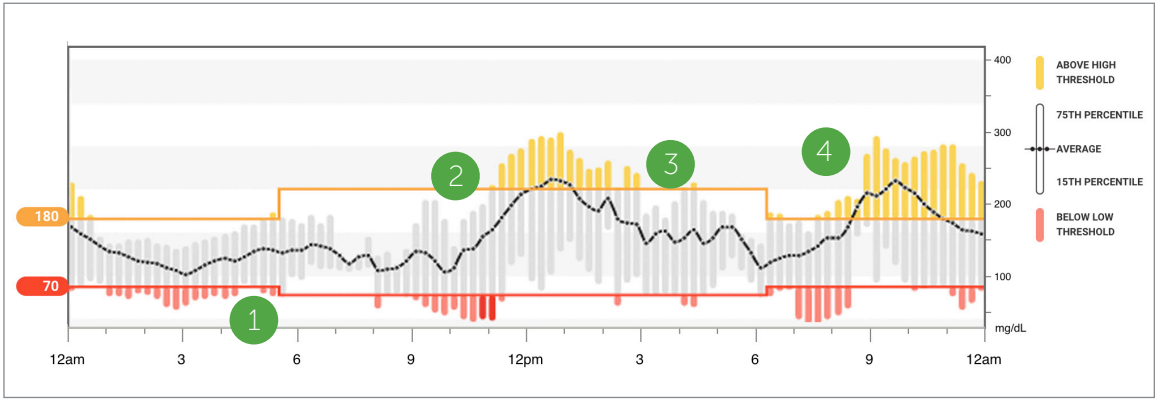

Glucose Pattern Management*

Dexcom CLARITY may not identify all clinical patterns. A stepwise approach may help you identify patient challenges with hypo- and hyperglycemia.

1. Hypoglycemia. Determine when hypoglycemia occurs and prioritize hypoglycemia overnight (1st) and hypoglycemia day/night (2nd). In this example the patient is experiencing overnight hypoglycemia (1st) as well as hypoglycemia during the morning and evening hours (2nd).

2. Pre-prandial glucose control. Determine if there is pre-meal hyperglycemia. In this example patient's lunchtime was at 11:00. No pre-prandial hyperglycemia is detected.

3. Post-prandial glucose control. Determine if there is post-meal hyperglycemia. In this example a pronounced post-prandial hyperglycemia is after lunchtime.

4. Overnight glucose control. Determine if there is overnight hyperglycemia. Appropriate levels of basal insulin should keep glucose values in target range throughout the night. This is a problem in the above example.

* Use your professional judgement when interpreting CGM data

Overlay Report

The Overlay features all CGM data points to help patients visualize patterns and individual events. Each line represents one day of data and each graph contains up to 7 days of all sensor data from the selected date range.

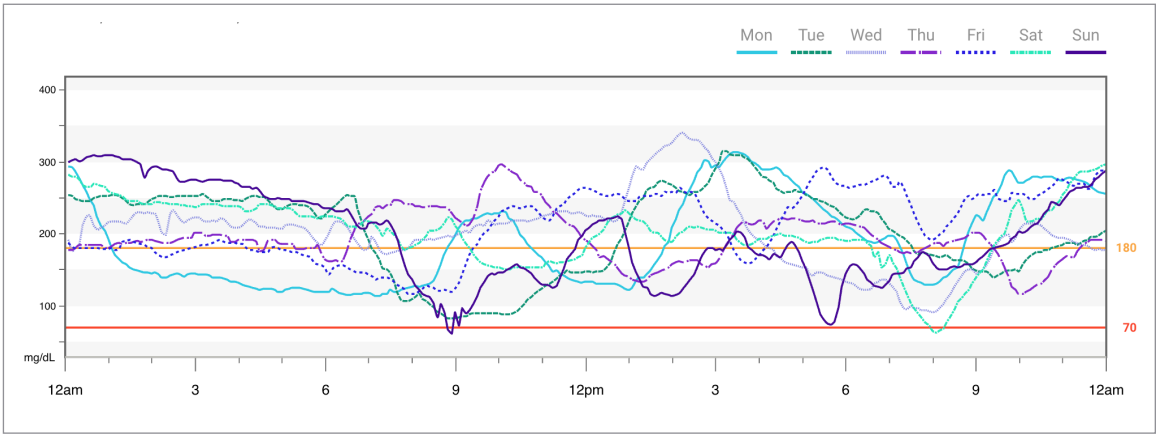

Customize reports by applying filters. View data by day of the week, day or night, lows and highs, rebounds, and sustained events. This can be useful to identify patterns of patients with irregular schedules.

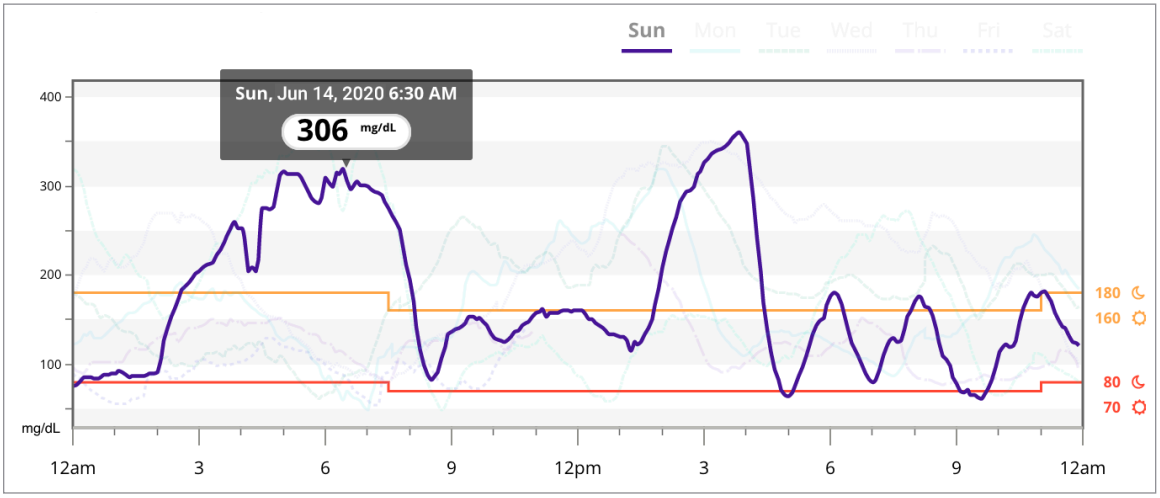

Daily Report

Use the Daily view to talk in depth with patients regarding individual days and isolated events. Every glucose reading is displayed in this report.

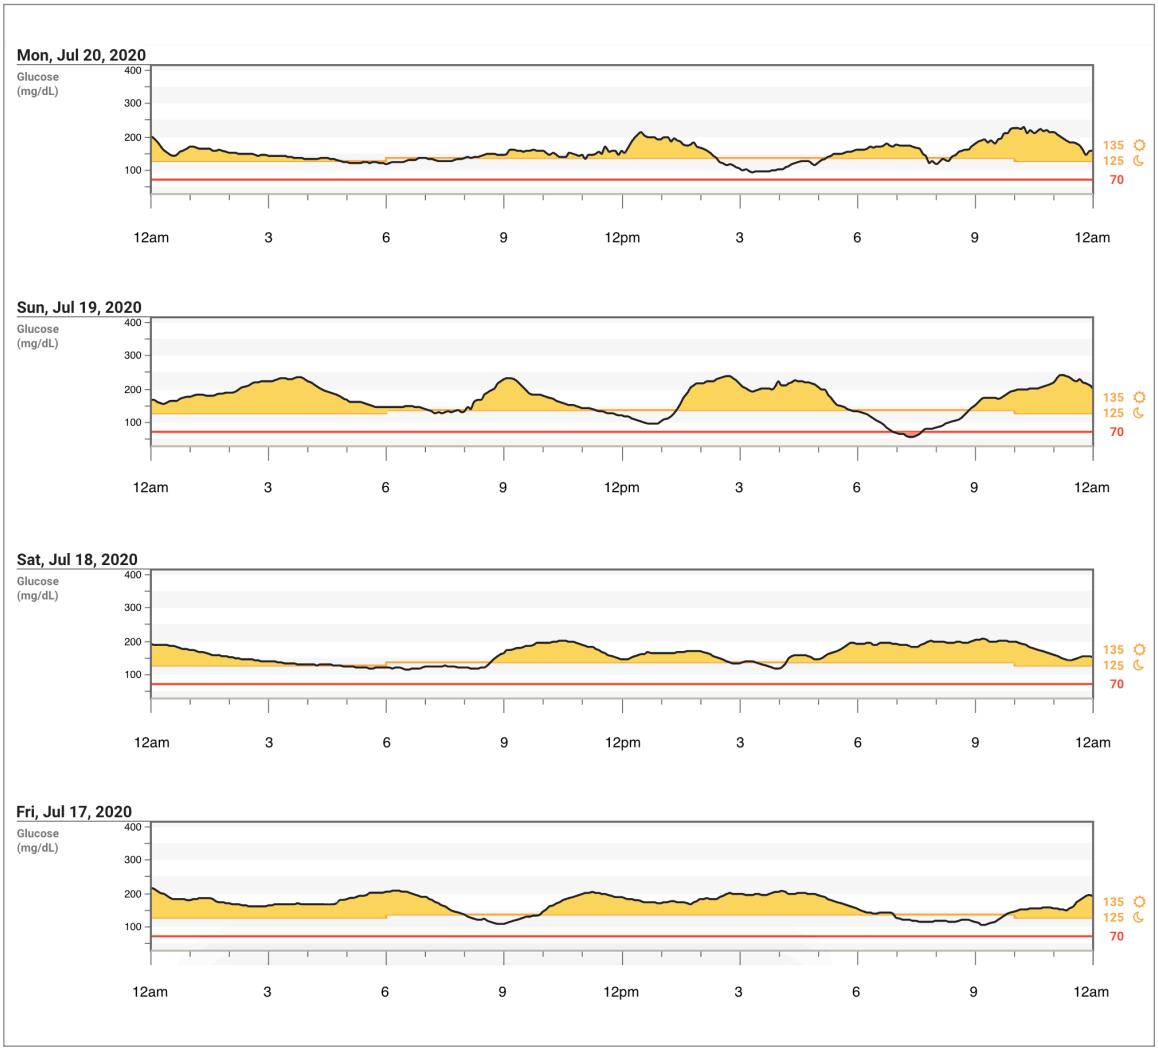

Compare Report

The Compare report encourages progress and highlights the challenges patients may be facing each visit. Review glucose changes from medication or dosage adjustments. Use during quarterly visits to pickup where you left off.

14 Days Tue Jun 23, 2020 - Mon Jul 6, 2020

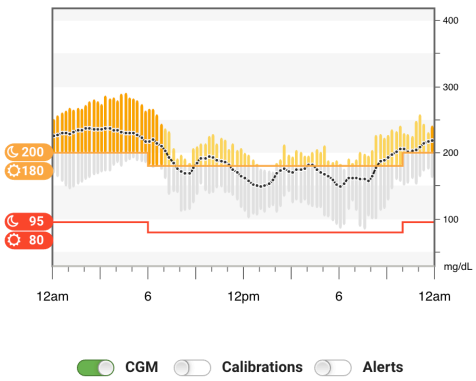

Statistics for this date range

Average Glucose

193 mg/dL

Standard Deviation

56 mg/dL

GMI

7.9%

Time in Range

16% Very High
38% High
45% In Range
1% Low
0% Very Low

Target Range: Day (6:00 AM - 10:00 PM): 80-180 mg/dL
Night (10:00 PM - 6:00 AM): 95-200 mg/dL

Sensor Usage

Days with CGM data

100%

14/14

Avg. calibrations per day

0.0

14 Days Tue Jul 7, 2020 - Mon Jul 20, 2020

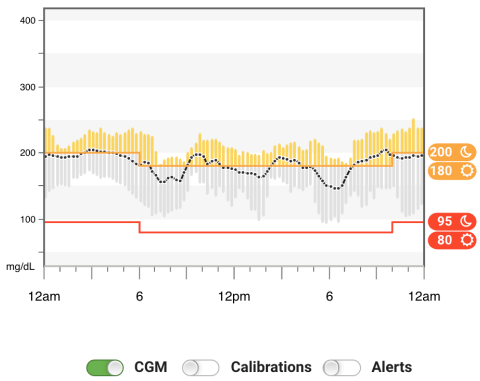

Statistics for this date range

Average Glucose

184 mg/dL

Standard Deviation

46 mg/dL

GMI

7.7%

Time in Range

6% Very High
42% High
50% In Range
1% Low
<1% Very Low

Target Range: Day (6:00 AM - 10:00 PM): 80-180 mg/dL
Night (10:00 PM - 6:00 AM): 95-200 mg/dL

Sensor Usage

Days with CGM data

93%

13/14

Avg. calibrations per day

0.0

Statistics Report

The Statistics report focuses on metrics and glucose control. Time in Range can be compared across days or times to identify issues.

Hourly statistics highlight each hour of the day, and can be used to detect patterns and fluctuations during overnight, daytime, or around a specific meal or event.

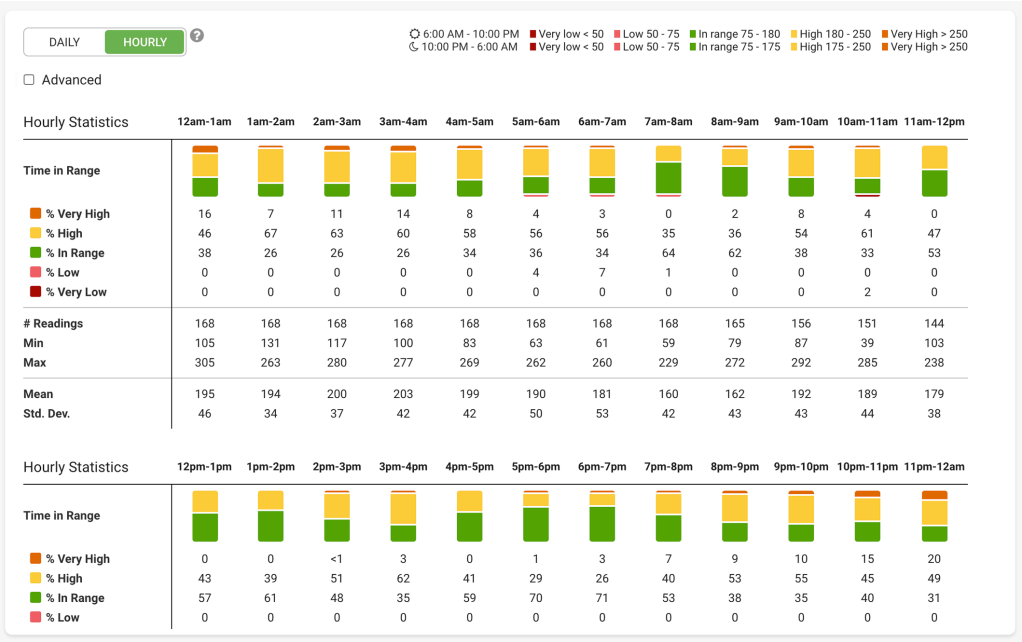

DAILY | HOURLY

Advanced

6:00 AM - 10:00 PM: Very low < 50, Low 50 - 75, In range 75 - 180, High 180 - 250, Very High > 250
10:00 PM - 6:00 AM: Very low < 50, Low 50 - 75, In range 75 - 175, High 175 - 250, Very High > 250

Hourly Statistics	12am-1am	1am-2am	2am-3am	3am-4am	4am-5am	5am-6am	6am-7am	7am-8am	8am-9am	9am-10am	10am-11am	11am-12pm
Time in Range												
% Very High	16	7	11	14	8	4	3	0	2	8	4	0
% High	46	67	63	60	58	56	56	35	36	54	61	47
% In Range	38	26	26	26	34	36	34	64	62	38	33	53
% Low	0	0	0	0	0	4	7	1	0	0	0	0
% Very Low	0	0	0	0	0	0	0	0	0	0	2	0
# Readings	168	168	168	168	168	168	168	168	165	156	151	144
Min	105	131	117	100	83	63	61	59	79	87	39	103
Max	305	263	280	277	269	262	260	229	272	292	285	238
Mean	195	194	200	203	199	190	181	160	162	192	189	179
Std. Dev.	46	34	37	42	42	50	53	42	43	43	44	38

Hourly Statistics	12pm-1pm	1pm-2pm	2pm-3pm	3pm-4pm	4pm-5pm	5pm-6pm	6pm-7pm	7pm-8pm	8pm-9pm	9pm-10pm	10pm-11pm	11pm-12am
Time in Range												
% Very High	0	0	<1	3	0	1	3	7	9	10	15	20
% High	43	39	51	62	41	29	26	40	53	55	45	49
% In Range	57	61	48	35	59	70	71	53	38	35	40	31
% Low	0	0	0	0	0	0	0	0	0	0	0	0

Daily statistics provides a basic daily visualization of percentage of highs, lows, and target.

DAILY | HOURLY

Advanced

6:00 AM - 10:00 PM: Very low < 50, Low 50 - 75, In range 75 - 180, High 180 - 250, Very High > 250
10:00 PM - 6:00 AM: Very low < 50, Low 50 - 75, In range 75 - 175, High 175 - 250, Very High > 250

Daily Statistics	Mon	Tue	Wed	Thu	Fri	Sat	Sun
Time in Range							
% Very High	3	17	9	0	3	2	7
% High	40	56	49	60	50	42	41
% In Range	52	27	42	40	47	55	51
% Low	5	0	0	0	0	0	<1
% Very Low	0	0	0	0	0	<1	0
# Readings	393	576	576	576	576	466	572
Min	61	124	95	82	77	39	59
Max	261	301	276	244	272	264	305
Mean	167	211	189	184	180	173	174
Std. Dev.	50	41	44	33	36	49	53
Quartile 25	131	175	159	159	158	135	133
Median	167	212	191	193	183	167	176
Quartile 75	214	240	225	206	202	219	218
IQR	83	65	66	47	44	84	85
IQ Std. Dev.	25	17	19	14	12	22	24
SD Mean	3	2	2	1	1	2	2
%CV	30	20	24	18	20	28	30

AGP Report

The Ambulatory Glucose Profile (AGP) is an American Association of Clinical Endocrinologists (AACE)-recommended standardized report for CGM interpretation created by the International Diabetes Center (IDC). This report show three distinct sections that:

1. Summarize glucose values to help assess the overall quality of glucose control.
2. Show variability around the mean glucose and patterned areas of highs and lows.
3. Show single-day glucose values to help identify patterns and progress.

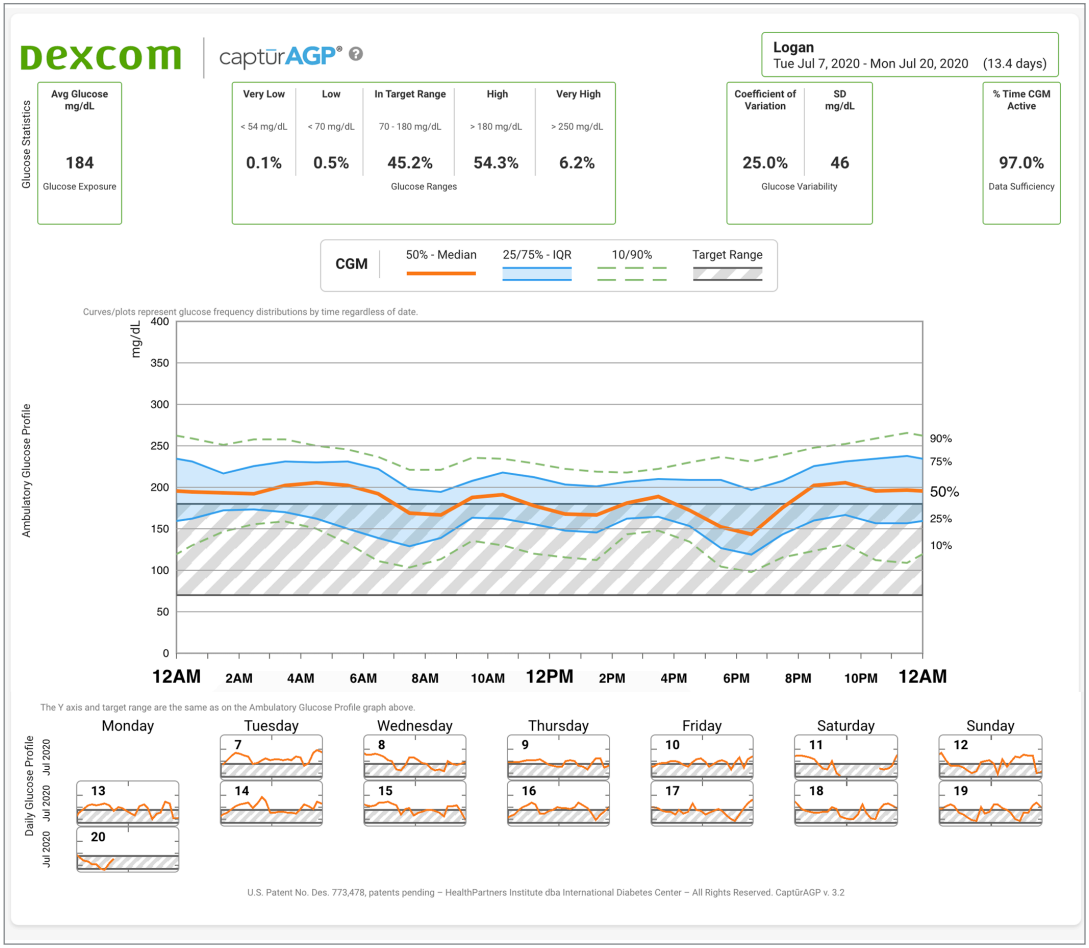

Pro Report

Patients wear the Dexcom G6 Pro for up to 10 days in blinded or unblinded mode. On the return visit, you can review the data from the Pro report to discuss session insights and make appropriate treatment recommendations. Then, you can submit the report for reimbursement for CGM setup and interpretation.

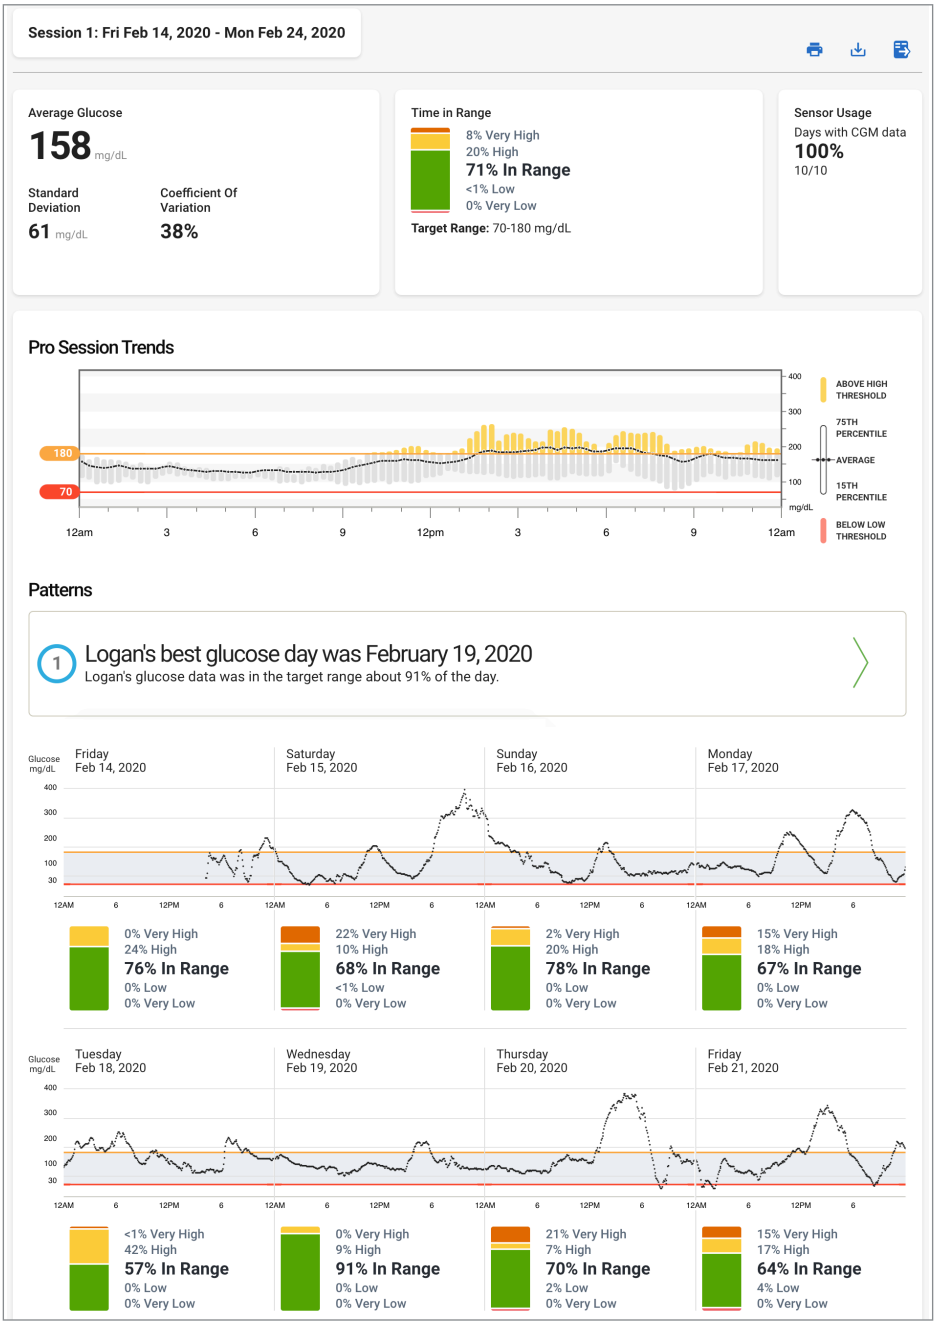

Save or Print Reports

All Dexcom CLARITY reports can be saved or printed for easy reference during patient visits.
When printed, this one page summary contains all information for billing 95251* which is a CPT code covered by most insurance carriers.

*95251: Ambulatory continuous glucose monitoring of interstitial tissue fluid via a subcutaneous sensor for a minimum of 72 hours; interpretation and report. (Do not bill more than once per month.)

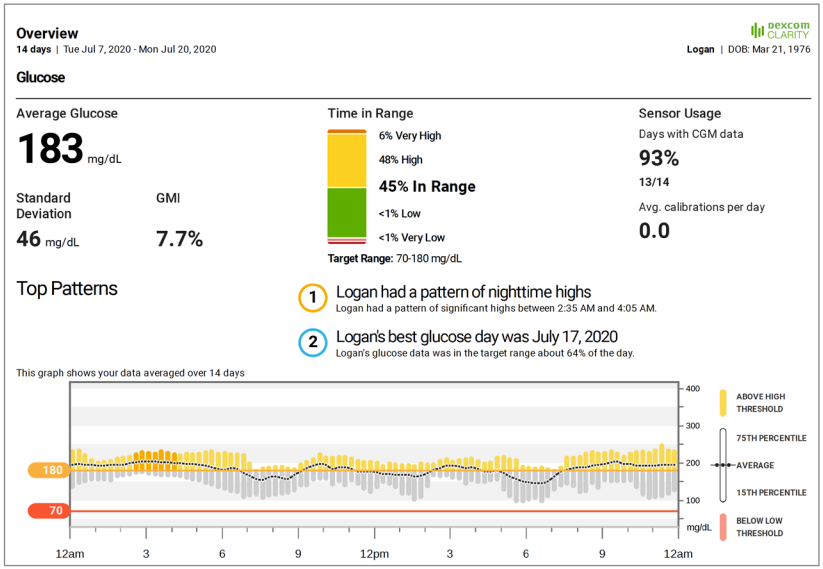

Patient Glucose Ranges

Use the Patient Glucose Ranges page to customize patient ranges for day and night.
Changes you make to a patient settings only apply at the clinic and do not change the patient's personal Dexcom CLARITY account or any CGM settings.
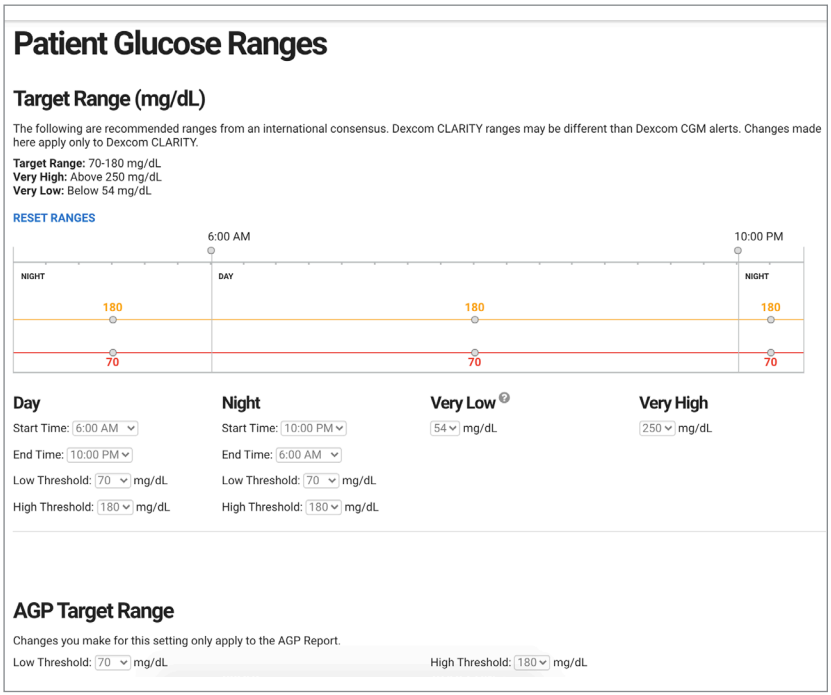
Reports are generated based on these settings.