

DCCT Test Results for DCCT S/N: DCCT-M-B-0022

Overall Test Status: Passed!

Technician: Kevin Mandracchia, Life #: 25337

Test performed: 03/22/25, 07:20 AM

Raw Serial Number/Sticker Data: DCCT-M-B-0022-22491031041-BZ22481532-HBA22410068B-22501031095-BZ22481966-HBA22190031-CTP-6303-50-

FLT12 Fault Signal 1 and 2 Test Results

| Test | Value | Status |
|------------------------------|---------|--------|
| FLT12 Overall Testing | N/A | Pass |
| FLT12 Positive Assertion | N/A | Pass |
| FLT12 Negative Assertion | N/A | Pass |
| FLT12 De-Assertion | N/A | Pass |
| FLT12 Initial Voltage | 14.77 V | Pass |
| FLT12 Positive Fault Voltage | 0.00 V | Pass |
| FLT12 Negative Fault Voltage | 0.00 V | Pass |

Pass/Fail Threshold Voltage for FLT12 Initial Voltage: >14.3V

Pass/Fail Threshold Voltage for FLT12 Fault Voltage: <1V

FLT12 Fault testing carried out with +/-1A current through DCCT

Test Current for IOUT Measurement: +/-10A at 10Hz Sinusoidal
(20Vpp sine into Kepco current control input)


Sinusoidal Current Test Results

| Test | Value | Status |
|--------------------------------|------------------|--------|
| CT Measurement Overall Testing | N/A | Pass |
| Channel 1 Voltage Threshold | 0.516Vpp | Pass |
| Channel 2 Voltage Threshold | 0.516Vpp | Pass |
| Channel 3 Voltage Threshold | 21.6Vpp | Pass |
| Frequency and Phase | 10.5 Hz, 180.01° | Pass |


Current Test Waveforms

ALSu DCCT Test Data


Channel 1, IOUT 1

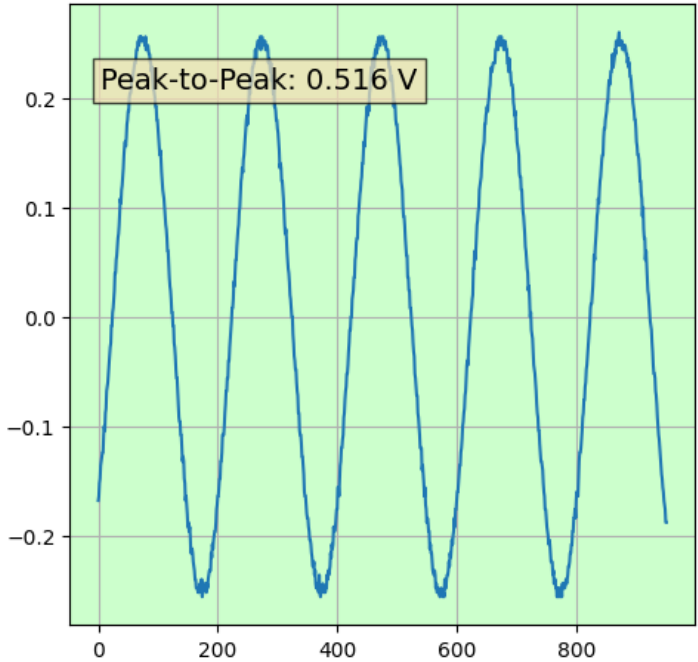

Channel 2, IOUT 2

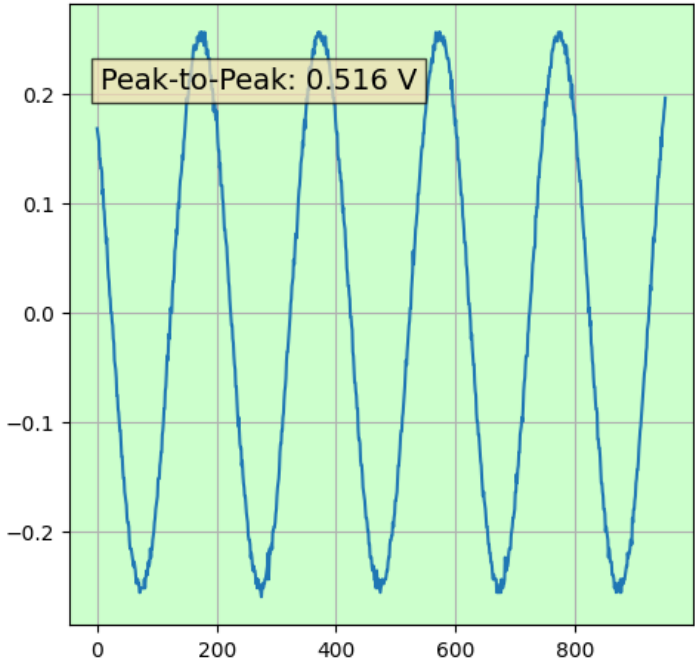

Channel 3, SIGNAL GEN

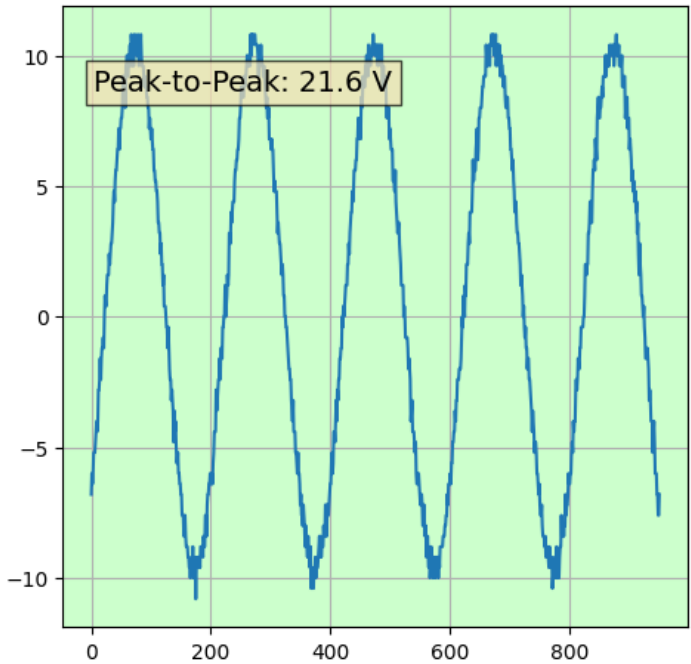

Channel 1 & Channel 2 (IOUT 1 and IOUT 2) Phase Shift

