NORTHLINE BENCH INSTRUMENTS

NB-410 Oscilloscope | Bench Measurement Report

MEASUREMENT REPORT

RESULT OUT OF SPEC

Serial no: NB410-579422
Report date: 12 Oct 2026
Calibration due: 12 May 2027
Tool: E-01
Chamber: E-01-A
Observed at: 2026-10-12T14:22:00Z
Instrument: oscilloscope
Parameter: rfPower
Plain name: RF power
Value: 2140
Unit: W
Spec minimum: 1000
Spec maximum: 2000
Shape: oscillation
Operator: KL
Specification: 1000 to 2000 W
Note: Peak-to-peak swing leaves the printed window.

TRACE RF POWER (W)

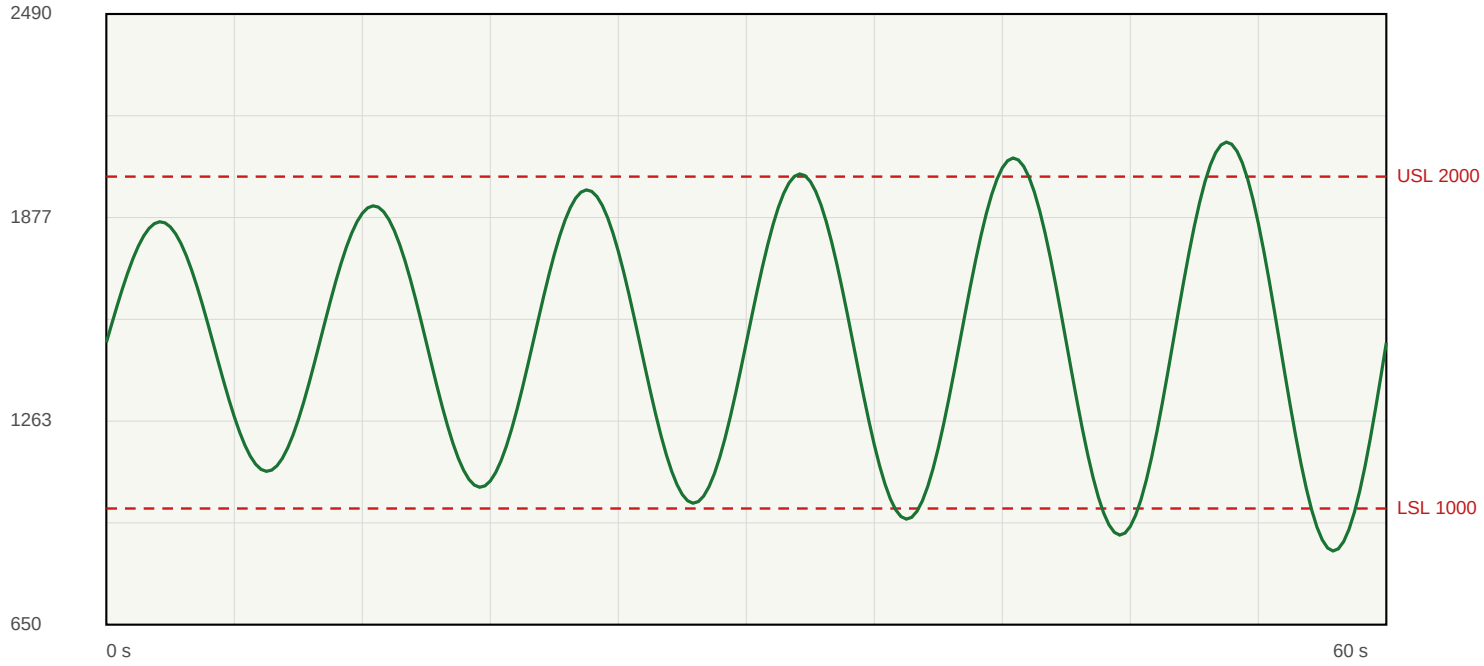

Channel	Measured	Min	Max	Result
RF power	2140 W	1000	2000	FAIL

Technician signature: _____ Initials KL

Reviewed by _____ Date _____