CALDER RIDGE METROLOGY

CR-220 RF power meter | Bench Measurement Report

MEASUREMENT REPORT

RESULT OUT OF SPEC

Serial no: CR220-550512
Report date: 12 Oct 2026
Calibration due: 12 May 2027
Tool: E-02
Chamber: E-02-A
Observed at: 2026-10-12T15:05:00Z
Instrument: rfPowerMeter
Parameter: rfBiasPower
Plain name: Bias RF power
Value: 510
Unit: W
Spec minimum: 200
Spec maximum: 500
Shape: step
Operator: MR
Specification: 200 to 500 W
Note: Forward power sits above the printed maximum.

TRACE BIAS RF POWER (W)

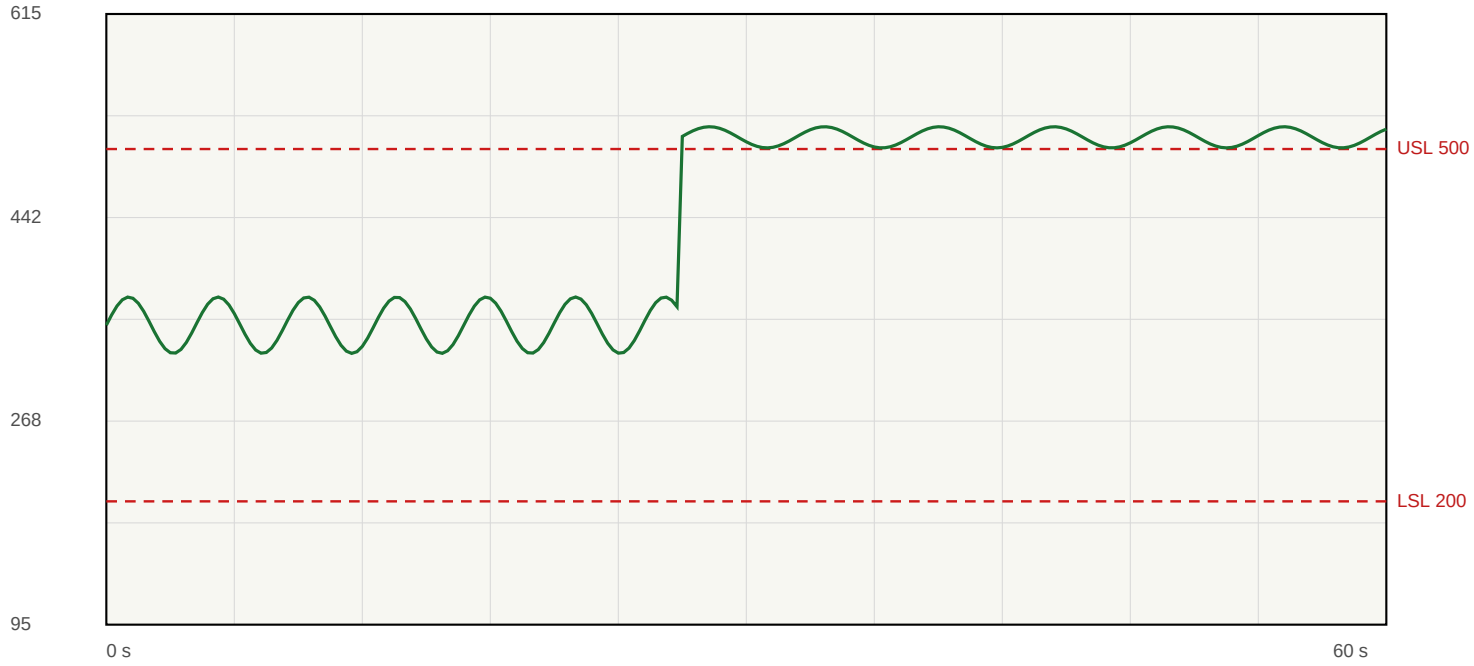

Channel	Measured	Min	Max	Result
Bias RF power	510 W	200	500	FAIL

Technician signature: _____ Initials MR

Reviewed by _____ Date _____