SABLE FORK INSTRUMENTS

SF-80 Thermocouple logger | Bench Measurement Report

MEASUREMENT REPORT

RESULT OUT OF SPEC

Serial no: SF80-667289
Report date: 12 Oct 2026
Calibration due: 12 May 2027
Tool: E-01
Chamber: E-01-A
Observed at: 2026-10-12T09:40:00Z
Instrument: thermocoupleLogger
Parameter: escTemperature
Plain name: ESC temperature
Value: 68
Unit: C
Spec minimum: 40
Spec maximum: 60
Shape: ramp
Operator: JL
Specification: 40 to 60 C
Note: The trace rises past the printed maximum.

TRACE ESC TEMPERATURE (C)

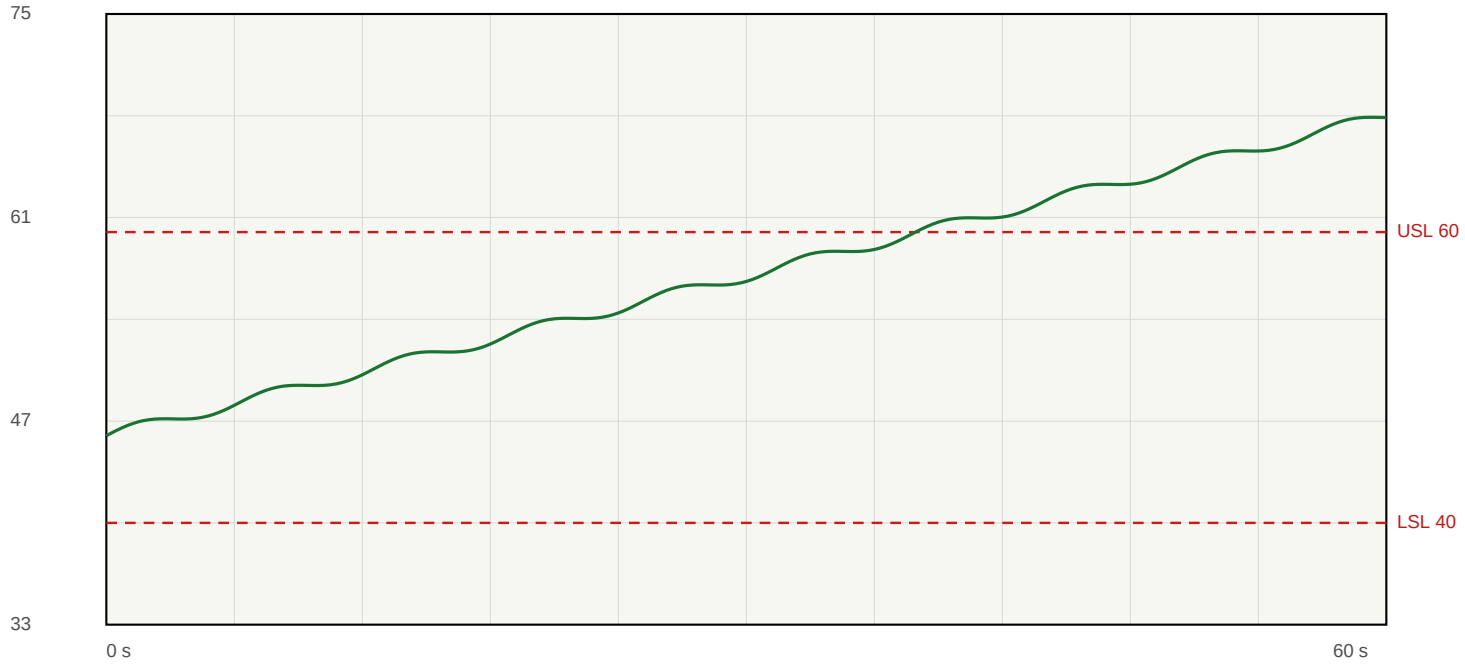

Channel	Measured	Min	Max	Result
ESC temperature	68 C	40	60	FAIL

Technician signature: _____ Initials JL

Reviewed by _____ Date _____