HEARTHLINE PARTICLE WORKS

HP-12 Particle counter | Bench Measurement Report

MEASUREMENT REPORT

RESULT OUT OF SPEC

Serial no: HP12-801533
Report date: 11 Oct 2026
Calibration due: 11 May 2027
Tool: D-01
Chamber: D-01-A
Observed at: 2026-10-11T18:10:00Z
Instrument: particleCounter
Parameter: particlesAdders
Plain name: Particle adders
Value: 18
Unit: count
Spec minimum: 0
Spec maximum: 10
Operator: BN
Specification: 0 to 10 count
Note: Adder count sits above the printed maximum.

PARTICLE SIZE DISTRIBUTION

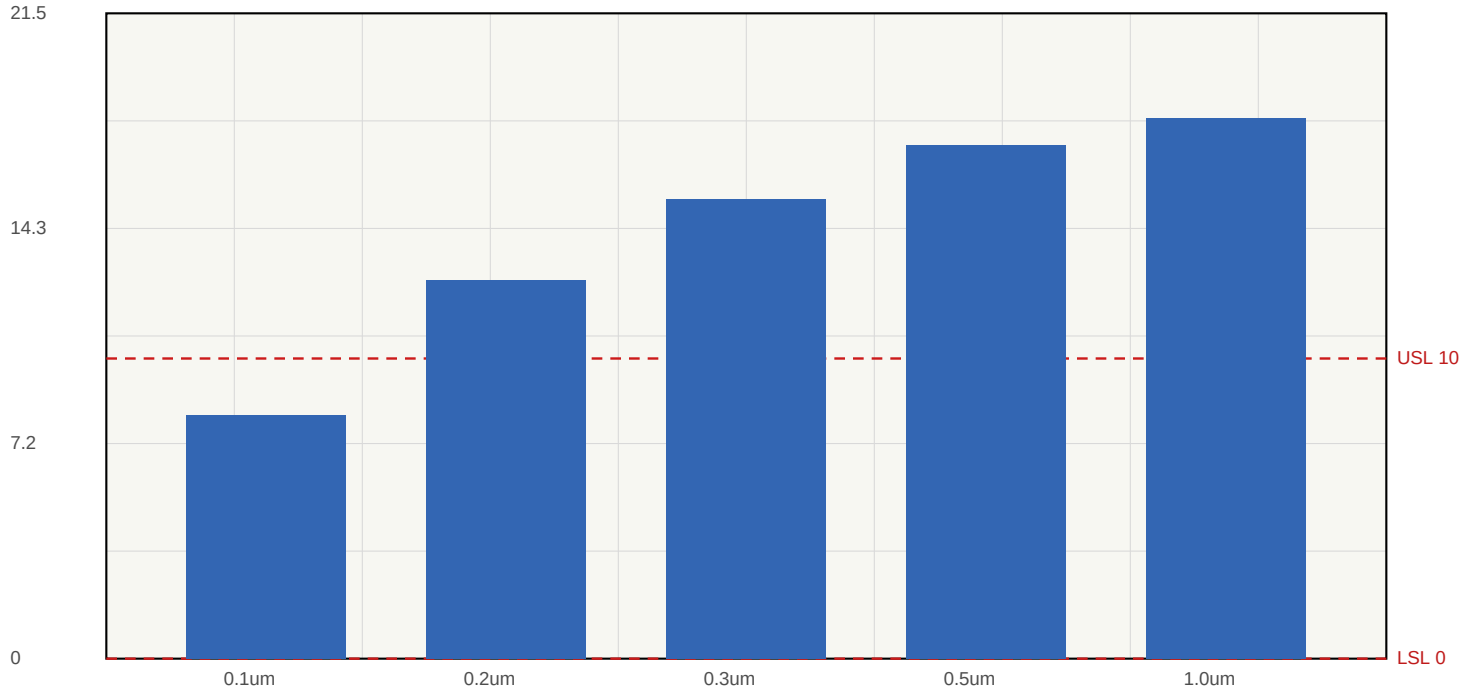

Cumulative adders per wafer, by particle size bin

Channel	Measured	Min	Max	Result
Particle adders	18 count	0	10	FAIL

Technician signature: _____ Initials BN

Reviewed by _____ Date _____