

# An Improved Transient Method for the Simultaneous Determination of Free-stream Reference Temperature and Convective Heat Transfer Coefficient:

## *The "Invariant $h$ Method"*

CENGİZ CAMCI

*The Pennsylvania State University, Department of Aerospace Engineering  
Turbomachinery Heat Transfer Laboratory,  
223 Hammond Building, University Park, PA, 16802*

**ABSTRACT :** This paper deals with the development of a new method that can provide heat transfer coefficient  $h$  and reference free stream temperature (adiabatic wall temp.) simultaneously by using the useful property that " $h$  does not vary in time when the mean flow conditions are stationary". The new "*invariant  $h$* " method can analytically determine local free stream temperatures in internal flow cases in which heat pick-up (or heat loss) is at a non-negligible magnitude. The method eliminates the need for cumbersome and error prone free stream gas temperature measurements using conventional sensors. The general method described in this paper is applicable to many different surface temperature mapping schemes that has a capability of measuring the surface temperature at each time step during a transient experiment. The mapping techniques in this category are discrete temperature sensors, infrared imaging and temperature sensitive paints (thermographic phosphors). An extension of the "*invariant  $h$* " method to "single shot" transient experiments can also be made for the direct determination of adiabatic wall effectiveness values in gas turbine cooling research using liquid crystal coatings.

## INTRODUCTION

Accurate determination of convective heat transfer coefficient requires a precise knowledge of the free stream reference temperature  $T_{o\infty}$  and the local temperature of the wall  $T_w$ . A better reference temperature for the gas stream is its corresponding "adiabatic wall temperature/recovery temperature"  $T_{aw}$ , Eckert<sup>1</sup>, Kays and Crawford<sup>2</sup>, Goldstein, Behbahani and Heppelmann<sup>3</sup>. Using adiabatic wall temperature as a reference temperature becomes more important in the compressible flow range where viscous dissipation is significant. The general method of finding  $h$  requires an accurate measurement of wall heat flux, reference temperature for the gas stream, and local wall temperature in both steady-state and transient methods. In many steady state methods, there are surface heater strips in the form of constant heat flux surfaces or isothermal wall strip heaters. The existence of any surface heater can increase the free stream gas temperature as one moves in the downstream direction of any heat transfer model. The free stream gas has the capability of

picking up non-negligible thermal energy from the wall. In the case of high speed flows, thermal energy produced via viscous dissipation mechanism may affect the local reference temperature of the free stream. In transient methods, the model is initially at a different temperature than that of the free stream fluid. Especially in internal flow cases such as serpentine cooling passages, pipes, ducts with small cross sectional area, heat pick-up (or heat loss) may be significant to alter the free stream reference temperature. One way to solve this problem is to instrument the passage in the streamwise direction so that the free stream reference temperatures are locally measured.

This paper describes an alternative method for the simultaneous determination of local  $h$  and  $T_{o\infty}$  (or  $T_{aw}$ ) in transient heat transfer experiments. The new concept introduced is capable of producing accurate local free stream reference temperatures without performing cumbersome gas stream temperature measurements using discrete sensors. Since the local free stream reference temperature is the same as the adiabatic wall temperature, the new method can be considered as a direct and accurate measurement method for the local adiabatic wall temperature.

The “*invariant h*” method presented in this paper is directly applicable to many surface temperature mapping methods including thin film sensors, thermocouples, thermistors, thermographic phosphors and infrared imaging. In the current study, the acquisition of local surface temperature at every time step starting from the beginning of the transient experiment is required. In this approach, a general wall temperature to heat flux conversion scheme allows a time dependent free stream reference temperature.

The same concept can also be implemented into more time efficient single shot experiments in which a single surface thermal image at a pre-selected time is acquired to obtain local  $h$  values by using an inverse solution of one dimensional transient heat conduction equation. This specific approach requires that the free stream reference temperature is constant in time. This method is preferred frequently because of its time efficiency and simplicity. Details of the modifications required to use the new “*invariant h*” method in a single shot experiment employing thermographic liquid crystal (TLC) coatings are not included in this paper. An accompanying paper by Camci<sup>4</sup> presents a detailed treatment of liquid crystal and film cooling related aspects of the new method.

## A BRIEF DESCRIPTION OF THE NEW “INVARIANT $h$ METHOD”

The convective heat transfer coefficient  $h$  assigned to a viscous layer existing between a free stream and a solid body is a strong indicator of the overall fluid dynamic status of the region. The definition of the convective heat transfer coefficient  $h = q_w / (T_{aw} - T_w)$  warrants the isolation of fluid dynamic effects from the thermal boundary conditions of the problem.  $h$  is only affected from the fluid dynamic features of the viscous flow layer. In a wide range of experimental conditions, the momentum equation and thermal energy equation are not coupled.

Any variation in the thermal driving potential ( $T_{aw} - T_w$ ) does not alter the magnitude of  $h$  provided that the local free stream Reynolds number is kept constant at a specific location. By definition,  $q_w$  is linearly dependent on ( $T_{aw} - T_w$ ) by the relation  $q_w = h(T_{aw} - T_w)$  as shown in Figure 1. When heat flux is plotted with respect to ( $T_{aw} - T_w$ ), the slope of the straight line is the local heat transfer coefficient. Therefore,  $h$  will always be the same regardless of the local heat flux  $q_w$  or the thermal driving potential value, provided that the free stream Reynolds number and turbulent flow character is kept unchanged at the specific location.

In a transient heat transfer experiment, either the free stream flow is started impulsively or the model is instantaneously injected into a steady stream. In both approaches, the flow related transients from the impulsive starting of the free stream or transients of model injection are kept to a minimum time duration when compared to the total elapsed time of the complete heat transfer experiment. The steady state flow conditions are reached rather quickly in most forced convection problems. The time scales of the viscous/turbulent diffusion of initial flow disturbances are usually much smaller than the total duration of the thermal transient created over the wall. In a typical transient experiment, time-wise change of the wall temperature is incorporated into an inverse solution of the transient heat conduction equation. It is possible to construct a “wall heat flux transient  $q_w(t)$ ” from a measured “wall temperature transient  $T_w(t)$ ” provided that the thermo-physical triple product  $\sqrt{\rho C_p k}$  of the solid body is known accurately. Many researchers in the past used this concept on heat transfer models that can be classified as semi-infinite bodies.

Once the initial flow disturbances decrease, the free stream Reynolds number at a selected point on the model remains constant over the complete duration of the experiment. This is a major assumption used in the development of the new method. There are currently many facilities operating in this mode either for gas side heat transfer or internal cooling passage heat transfer research. Flow and heat transfer characteristics of the most typical of these facilities can be found in Camci, Kim, Hippensteele and Poinsette<sup>5</sup>, Jones and Hippensteele<sup>6</sup>, Ireland and Jones<sup>7</sup>, Metzger, Bunker and Bosch<sup>8</sup>, Vedula and Metzger<sup>9</sup>, Ekkad and Han<sup>10</sup>, Drost, Hoffs and Bolcs<sup>11</sup>.

Previously, the determination of the reference temperature of the free stream was mainly an experimental temperature measurement performed at a fixed point in the free stream. The number of studies documenting the variation of the reference free stream temperature in the streamwise direction is limited. The present method eliminates the need to obtain reference free stream temperature  $T_\infty$  (or  $T_{aw}$ ) by an independent experimental method. Since the local Re number is constant in a typical transient experiment, the local convective heat transfer coefficient  $h$  is supposed to remain constant in time. By using this “*invariant h*” property in addition to the transient conduction equation at the fluid-solid interface, one can easily obtain  $h$  and  $T_{aw}$  “*simultaneously*”. This new approach is extremely powerful in heat transfer problems where heat pick-up (or heat loss) of the free stream gas is measurable in magnitude. The present study shows that the new “*invariant h*” property is extremely useful in finding the reference gas temperature or adiabatic wall temperature analytically by eliminating extra experimental efforts and errors. The new method is completely analytical and allows the researcher to obtain the local free stream reference temperature at every point where a transient wall temperature measurement is possible. The accurate level of the free stream reference temperature is reached by forcing the local convective heat transfer coefficient  $h$  in time to a time-wise stationary status in an iterative process.

### GENERIC TRANSIENT TEST CASE DEFINITION

It is essential to explain the new method using a generic transient heat transfer test case that is applicable to most forced convection heat transfer studies. An impulsively starting flow is established over a flat plate in a few milliseconds time. The heat transfer coefficient  $h$  under these conditions is assumed to be  $100 \text{ W/m}^2\text{K}$ . The free stream reference temperature at the edge of the boundary layer is constant at  $T_\infty = T_{aw} = 302^\circ \text{K}$  over the duration of the transient test that lasts about 8 seconds. It is prescribed that the model is kept at  $283^\circ \text{K}$  initially. Time-wise change of the wall temperature  $T_w(t)$  recorded by a wall sensor at the specific  $x$  location is shown in

Figure 2. This temperature rise also satisfies Equation 1 for  $h=100 \text{ W/m}^2\text{K}$ . The model wall thickness satisfies the conditions required for being considered as semi-infinite. The thermo-physical triple product for the plexiglass model material is about  $\sqrt{\rho C_p k} = 569 \text{ W} \cdot (\text{sec})^{1/2} / \text{m}^2$ . Figure 2 also shows a reconstructed wall heat flux trace  $q_w(t) = h(T_{aw} - T_w(t)) = 100 \cdot (302 - T_w(t))$  using a one-dimensional transient heat transfer (inverse) solution for a semi-infinite body, (equation 1). The heat flux  $q_w(t)$  to the wall decrease in time because of the temperature rise at the fluid-solid interface. The corresponding heat transfer coefficient for this ideal case can be re-calculated from  $h(t) = q_w(t) / (T_{\infty} - T_w(t))$ . When  $h$  is re-calculated from  $q_w(t)$  and  $T_w(t)$  shown in Figure 2, a constant value of  $100 \text{ W/m}^2\text{K}$  over the complete duration of the transient test is obviously obtained. The heat transfer coefficient  $h$  is an invariant quantity in a transient test where free stream  $Re_x$ ,  $Tu_{\infty}$  and  $T_{aw}$  are constants in time:

### TYPICAL UNCERTAINTY OF $h$

In the measurement of  $h$ , the errors made in wall temperature, reference free stream temperature and wall heat flux all contribute to  $\delta h$  at different rates. However, the most significant error contributor seems to be the reference free stream temperature as shown in Figure 3. Figure 3 represents the best measurement quality in terms of the wall temperature error,  $\delta T_w = \pm 0.1^\circ \text{K}$ . The figure shows the relative error on heat transfer coefficient  $\delta h/h$  in function of the reference free stream temperature error,  $\delta T_{\infty}$  (or  $\delta T_{aw}$ ). The relative error in  $h$  has a tendency to increase approximately 10 fold when the error in the measurement of the reference free stream temperature  $\delta T_{aw}$  is increased from  $\pm 0.1^\circ \text{K}$  to  $\pm 2^\circ \text{K}$ . A similar error increasing trend (with increasing  $\delta T_{aw}$ ) exists for the wall heat flux methods having higher error levels (e.g.  $\delta q_w/q_w = \pm 8\%$ ), however the relative error levels ( $\delta h/h$ ) are much higher as indicated by the dashed line in Figure 3.a.

Similar trends exist for a mediocre wall temperature measurement ( $\delta T_w$  5 times higher compared to the previous figure) effort that has an uncertainty of  $\delta T_w = \pm 0.5^\circ \text{K}$ . The same conclusions as the previous case can be drawn, however overall relative error  $\delta h/h$  follows a more elevated uncertainty character. The main result from this error analysis is that the most significant contributor to the error made in the determination of heat transfer coefficient  $h$  results from the uncertainty on "reference free stream temperature" ( $\delta T_{\infty} = \delta T_{aw}$ ). The relative contribution of various error sources in total error is plotted in the form of individual error norms in Figure 4. After a limiting value of  $\delta T_{aw} = \pm 0.6^\circ \text{K}$ , the contribution of reference free stream temperature measurement exceeds the errors made in the measurement of wall heat flux ( $\delta q_w/q_w$ ). Wall temperature measurement errors are actually a small part of the total error on  $h$  as shown in Figure 4. The error analysis presented in Figures 3 and 4 clearly justifies the need for a better method to obtain local reference gas temperatures over a heat transfer model.

### DETAILS OF THE "INVARIANT $h$ " METHOD

A hypothetical test case having a free stream reference temperature of  $302^\circ \text{K}$  produces  $h=100 \text{ W/m}^2\text{K}$  at a selected streamwise location of a heat transfer model. The model has a uniform initial wall temperature of  $283^\circ \text{K}$  and the free stream total temperature remains constant in time after the initial transients. The wind tunnel is operated such that the Reynolds number and free stream turbulence intensity at the specific measurement location is consistent with the targeted  $h$  value

of 100 W/m<sup>2</sup>K. The corresponding wall temperature rise from this test is shown in Figure 2. Finding an accurately representative  $T_w(t)$  profile that will generate  $h=100$  W/m<sup>2</sup>/K (constant in time) at a selected location can be achieved by using a simplified inverse solution of the transient heat conduction equation. For this case, the wall temperature transient, in the form of a non-dimensional wall temperature, can be related to heat transfer coefficient  $h$ , time and the free stream reference temperature by equation 1

$$\frac{T_i - T_w(t)}{T_i - T_{\infty}} = 1.0 - \exp(\beta^2) \cdot \text{erfc}(\beta) \quad (1)$$

where  $\beta = h\sqrt{t}/\sqrt{\rho C_p k}$  is non-dimensional time. The wall temperature profile plotted in Figure 2 has been obtained from equation 1 by using the specified values of  $T_i$ ,  $T_{\infty}$  and  $\sqrt{\rho C_p k}$ . Figure 2 also shows the corresponding wall heat flux  $q_w(t)$  variation obtained by multiplying the specified  $h=100$  W/m<sup>2</sup>K by the thermal driving potential  $[T_{\infty} - T_w(t)]$ . Equation 1 is usually preferred in single shot experiments in which a wall temperature measurement is required at one user selected time during the transient. This method is suitable for liquid crystal based wall temperature measurements. Although extremely simple, equation 1 can not handle the cases in which there are free stream reference temperature variations in time. Equation 1 has only been used to find a baseline wall temperature profile that will be used for further development of the “*invariant h*” method. The new method will be explained and validated for the general case in which the free stream reference temperature can vary in time.

The instantaneous wall heat flux  $q_w(t)$  in the “*invariant h*” method can also be re-constructed from  $T_w(t)$  by using a convolution integral solution that can be obtained by Laplace transforming the transient heat conduction equation. For general applications in which reference free stream temperature may vary in time, the final inverse solution to 1-D transient heat conduction equation from Schultz and Jones<sup>12</sup> can be written as follows.

$$q_w(t) = \sqrt{\rho C_p k / \pi} \left\{ \frac{T_w(t)}{\sqrt{t}} + \frac{1}{2} \int_{\tau=0}^t \frac{T_w(t) - T_w(\tau)}{(t - \tau)^{3/2}} \cdot d\tau \right\} \quad (2)$$

Equation 3 shows a more computationally efficient form of equation 2 that can be obtained via a series summation of delayed ramp functions, as suggested by Oldfield, Jones and Schultz (1978)<sup>13</sup>.

$$q_w(t) = q_w(m\Delta\tau) = \frac{2 \cdot \sqrt{\rho C_p k}}{\sqrt{\pi \Delta\tau}} \sum_{n=0}^m (T_{n+1} + T_{n-1} - 2T_n)(m - n)^{1/2} \quad (3)$$

The heat flux trace  $q_w(t)$  re-constructed from the wall temperature transient  $T_w(t)$  using the “general method” leading to equation 2 is shown in Figure 2. From this point on, the identical methods described in equations 2 and 3 will be termed as the “general method” for wall temperature to heat flux conversion. At this point, a perturbation experiment can be performed numerically in order to see what happens to  $h$  in time when “*perturbed*” reference free-stream temperature values are substituted into  $h(t) = q_w(t)/(T_{\infty} - T_w(t))$ . Figure 5 shows a number of  $h(t)$  curves calculated for the disturbed values of  $T_{\infty}$ . What happens to  $h(t)$  from this point on is nothing to do with neither the quality of  $T_w$  measurement nor  $q_w$  calculation using equation 2. Instead of  $T_{\infty}$ , Figure 5 uses [FACTOR $\times T_{\infty}$ ] in the equation for  $h$ . The product [FACTOR $\times T_{\infty}$ ] is also termed as the “*suggested free stream temperature*” during the iterative process. The value of FACTOR has been varied from 0.970 to 1.050 with small increments of 0.001.

Of course, when FACTOR is exactly 1.000, a time invariant heat transfer coefficient  $h$  is clearly established for all times as shown in Figure 5. The most

interesting observation is made when the distortion is at its strongest level. For  $FACTOR=0.99$ , the resulting  $h(t)$  values, have of course wrong absolute values. However the most valuable observation is that  $h(t)$  curve is not anymore invariant in time. The only time  $h(t)$  has a zero slope is when the correct reference free stream temperature is used in equation 2. This is an extremely useful property that repeats itself in every forced convection heat transfer experiment in the same fashion. When the perturbation parameter  $FACTOR$  goes to values greater than 1.000, the same observation is valid however, the slope of  $h(t)$  curve is negative. To determine “*if the suggested  $FACTOR \cdot T_{\infty}$  value is proper ?*” for the specific measurement, it is sufficient to monitor if a sign change in the slope of  $h(t)$  curve occurs from one perturbation value to another one. In a transient experiment, after one records a  $T_w(t)$  trace and construct  $q_w(t)$ , one may suggest a set of reference free stream temperature values that are perturbed around an expected value. Monitoring the slope of  $h(t)$  curve and forcing it to zero, one may find the exact actual free stream reference temperature at this specific location. The new approach described is analytical and replaces conventional  $T_{\infty}$  measurement efforts that usually introduce additional experimental errors. Figure 5 shows the extremely sensitive nature of the overall slope of  $h(t)$  curve to variations in  $FACTOR$ .

In summary, the “*invariant h*” method is about systematically varying an estimated “reference gas temperature” in the equation for  $h$  and numerically determining the overall slope of  $h(t)$  curve for each suggested gas temperature value ( $FACTOR \cdot T_{\infty}$ ). The numerical process is fast and efficient. The goal is to minimize the slope of  $h(t)$  curve down to a zero value during an iterative process. The same procedure can also be performed by monitoring if a sign change occurs in the overall slope of  $h(t)$  curve. Since most  $h(t)$  curves are highly linear, the test can be successfully performed over a short time interval near the end of the transient test. The sign change occurs only when a correct reference free stream temperature is used. It is also apparent from Figure 5 that the most accurate heat transfer coefficient is obtained only when  $h$  is invariant in time.

A different presentation of the same concept is given in Figure 6 by monitoring the local change in heat transfer coefficient at every time step. The local time-wise change in  $h$  was plotted with respect to time. The same data shown in Figure 5 is just plotted in a different form. However, the variation of the local slope for various  $FACTOR$  values is more visible in this form. The zero approaching feature of local slope at any time point is obvious when  $FACTOR$  is incrementally varied.

Figure 7 presents the relationship between “resulting” heat transfer coefficient and its time-wise slope at the end of the transient run for each suggested free stream temperature value. Monitoring the heat transfer coefficient against its slope is certainly a very effective method for isolating the correct free stream temperature and its associated heat transfer coefficient. When  $FACTOR$  varies from a low (0.970) to a high value (1.030) by an increment of 0.001, whenever a slope value of zero is reached, the correct  $h$  value and its associated free stream temperature is obtained. The use of  $FACTOR$  in this generic case was only permitted for testing the character of the suggested method. In laboratory applications, instead of using ( $FACTOR \cdot T_{\infty}$ ) one may start testing the slope of heat transfer variation by using a suggested starting value for the reference temperature of the free stream. The choice of the starting value is straight forward because the researcher have always the knowledge of an approximate free stream temperature. For example, in a transient test to be performed in a pedestal type cooling passage the inlet value of the free stream gas is more than sufficient to start the iterative process. Further examination of the relationship between  $h$  and its slope shows that the (almost) second order curve

as shown in Figure 7 can be linearized by normalizing the slope using the  $h$  value at the end of the transient run when  $t=t_f$ . For this case, a new quantity  $\Gamma$  showing the status of the slope of  $h$  is defined as  $\Gamma = \{\text{SLOPE}/h(t_f)\} * 100$ . Figure 8 presents data from the last 5 points of the generic transient experiment summarized in Figure 2. Isolating the correct  $h$  and its associated "reference free stream temperature" is a matter of finding the proper level of suggested free stream temperature that is corresponding to  $\Gamma=0$  in a simple iterative process. The trial is the suggested free stream temperature, and the error is the finite level of  $\Gamma$ . By forcing error  $\Gamma$  to zero, the heat transfer coefficient and reference temperature of the free stream can be obtained simultaneously and accurately. All five points at the end of the transient run provided the same functional dependency as shown in Figure 8. Using just one of the five points in Figure 8 is sufficient to obtain the correct  $h$  and its associated "reference free stream temperature".

### SUGGESTED PROCEDURE AND APPLICATION OF THE METHOD

The suggested numerical procedure summarizing the "invariant  $h$  method" that can be easily built into a computer procedure. A wall temperature transient is recorded by known methods of non-intrusive measurement techniques such as flush mounted thermocouples, thin film resistance sensors, thermistors, infrared imaging and thermographic phosphors emitting laser induced fluorescence. The general method described here requires the capturing of the complete transient in wall temperature with uniform time step  $\Delta\tau$ . The next step is to convert the measured  $T_w(t)$  to  $q_w(t)$  by using either Equation 2 or 3. It should be noted that these two equations allow the user to work with reference free stream temperatures that may actually vary during the transient experiment. The only condition to be satisfied here is the maintenance of constant free stream Reynolds number at the measurement location. Since most transient heat transfer facilities are designed with stationary free stream flow conditions in mind, this is a realistic and straight-forward condition to satisfy. After constructing the wall heat flux transient a starting suggested value for the free stream temperature is needed. A rough guess on this value is sufficient to start the trial and error procedure. In most facilities, the free stream temperature measured at the inlet of the test section is a good enough starting value. For example in a transient test in which the model is initially heated, as one moves along the streamwise direction, the free stream temperature at the edge of the boundary layer at different locations may vary because of different heat pick up rates from the heated model surface. When the model is cooled by the relatively colder free stream air, thermal energy is absorbed by the free stream. For this case, starting from the test section inlet value of free stream temperature and increasing the suggested value at each step by about 0.001 times the value of the initial guess may allow the user apply the procedure described in Figure 8. The incremental change needs to be sufficiently small so that the sign change of the normalized slope  $\Gamma$  can be detected with sufficient resolution. The process of incrementally varying "suggested" free stream temperature continues until a zero slope (or a sign change) is detected. At this point the resulting  $h$  and the suggested free stream temperature are recorded as the final measurement results.

### EXPERIMENTAL CONFIRMATION OF THE NEW "INVARIANT $h$ METHOD"

The specific method described in this paper is based on the observation that a wrong determination of the free stream reference temperature can cause a significant

error in the calculation of heat transfer coefficient  $h$  although the wall heat flux and wall temperature is measured properly. There are two excellent examples of this observation in the literature by Goldstein and Behbahani<sup>15</sup> and Kim<sup>16</sup>. They used a heated impinging jet impinging to a flat plate initially kept at ambient temperature. Although the round jet is heated in this case, the surrounding still air is at ambient temperature.

A schematic of our current transient heat transfer experiments performed for this arrangement at  $Re=30,000$  based on the jet diameter (nozzle exit) and velocity is shown in Figure 9. It is obvious that the entrainment of the cold surrounding air to the heated jet tends to cool the fluid in the wall jet layer as the jet fluid moves toward the impingement plate. The heating potential of the wall jet is also reduced when one moves away from the stagnation point in radially outward direction. The heating potential may even disappear far away from the stagnation region by the cooling influence of the entrained fluid. The past studies clearly showed that the heating potential for this problem should be considered as the temperature difference ( $T_{rec}-T_w$ ) instead of ( $T_{jmax}-T_w$ ) especially when the jet temperature at the nozzle exit  $T_{jmax}$  is different from the surrounding fluid temperature in still air. The correct reference temperature  $T_{ref}$  for the free stream is the recovery (adiabatic) temperature of the wall at a specific radial position on the impingement plate. The measurement of the adiabatic temperature of the wall at infinitely long time after the start of a transient experiment is sufficient to find  $T_{rec}=T_{aw}$ . It is important to wait for a long duration (at least an hour for the present experiment) to reach adiabatic conditions on the impingement plate during the acquisition of  $T_{aw}$ . It should be noted that during a transient experiment although the wall temperature increases in time, the reference temperature of the free stream (the edge of the wall jet fluid) is in steady state at a level of  $T_{ref}=T_{aw}$ .

What happens to Nusselt number (or  $h=Nu.k/D$ ) when one uses the wrong free stream reference temperature is shown in Figure 10 for  $H/D=6$ . The distribution shown as  $Nu'$  is obtained from a transient heat transfer experiment using nozzle exit temperature  $T_{jmax}$  as free stream reference temperature. The same value of  $T_{ref}=T_{jmax}$  was used for all radial positions on the impingement plate. The distribution denoted as  $Nu$  is for the case in which a measured local adiabatic wall temperature is used for each radial position as reference free stream temperature. The difference between measured local  $Nu$  and  $Nu'$  can be very large as shown in Figure 10. At  $r/D=2.4$ , the the measured (correct) heat transfer coefficient  $h=Nu.k/D$  can be as high as 300 % of corresponding  $h'=Nu'.k/D$  obtained with  $T_{jmax}$ . The difference between  $Nu$  and  $Nu'$  is monotonically reduced when one moves radially inward toward the stagnation point. Of course entrainment of cold surrounding air into the heated jet fluid is much more significant at outer radius locations than the stagnation point. At the stagnation point  $Nu$  is about 20 % higher than  $Nu'$ . The experiments clearly show the amount of energy lost into relatively cold still air from the heated wall jet needs to be taken into account. When a wrong free stream reference temperature is used in a transient experiment significant errors may be introduced into heat transfer coefficient distributions as shown in Figure 10.

The transient heat transfer data shown in Figure 10 also show a second interesting feature. The impinging jet experiment is executed by using a nozzle exit flow that is in steady state after an extremely short time duration (a few milliseconds). The total duration of the transient experiment is about 90 seconds. The heat transfer coefficient  $h$  is supposed to be "invariant" in time during the whole duration of the transient experiment. Although the wall temperature has a strong transient, the hydrodynamic conditions in the viscous flow zone need to be invariant in time. When the reference temperature is taken as  $T_{jmax}$ , not only the measured



heat transfer coefficient levels are wrong, they also have strong time dependency. It is interesting to note that when measured local adiabatic wall temperature is used as  $T_{ref}$ , time dependency of  $h=Nu.k/D$  can be eliminated. The observations made up to this point form an experimental confirmation of the "*invariant h*" method presented in this paper. By using the fact that  $h$  remains invariant during a transient experiment one can simultaneously obtain the local reference temperature belonging to free stream fluid by forcing the time-wise slope of  $h$  to zero.

## CONCLUSIONS

This paper deals with the explanation of a new method for the simultaneous and accurate determination of the convective heat transfer coefficient  $h$  and the corresponding reference free stream temperature.

The new "*invariant h*" method can analytically determine local free stream reference temperatures in internal flow cases in which heat pick-up (or heat loss) is at a non-negligible magnitude. The method is based on the useful property that " $h$  does not vary in time when the mean flow conditions are stationary" in a transient heat transfer experiment where free stream flow conditions are stationary..

The method eliminates the need for cumbersome and error prone free stream gas temperature measurements using conventional sensors. The general method described in this paper is applicable to surface temperature mapping schemes that has a capability of mapping the surface at each time step during a transient experiment.

The new method is extremely useful in internal and external flow configurations in which the free-stream reference temperature is continuously modified by a heated wall or a heated free stream.

The same concept can also be implemented into more time efficient single shot experiments in which a single surface thermal image at a pre-selected time is acquired to obtain local  $h$  values by using an inverse solution of one dimensional transient heat conduction equation. Details of the modifications required to use the new "*invariant h*" method in a single shot experiment employing thermographic liquid crystal (TLC) coatings and the applications of the method in finding adiabatic wall temperature (or effectiveness) in film cooling research is not included in this paper. An accompanying paper by Camci<sup>4</sup> presents a detailed treatment of liquid crystal and film cooling related aspects of the new method.

## ACKNOWLEDGMENTS

This investigation would not have been possible without a faculty fellowship granted by the AGTSR (Advanced Gas Turbine Systems Research) of South Carolina Institute for Energy Sciences (SCIES). The program monitor for the fellowship was Dr. Daniel Fant of AGTSR. Acknowledgements are also due to Dr.R.Bunker of GE Schenectady who acted as the industrial monitor of the AGTSR faculty fellowship. The author would like to thank to S.A.Hippensteele and Dr.R.Gaugler of the Turbine Branch of NASA Glenn Research Center for their valuable support during the initial phase of this study.

## REFERENCES

1. Eckert, E.R.G. 1959. Heat and Mass Transfer. McGraw Hill Book Company Inc. New York, NY.
2. Kays, W.M. & M.E.Crawford. 1980. Convective Heat and Mass Transfer. McGraw Hill Book Company Inc. New York, NY.

3. Goldstein, R.J., A.I.,Behbahani and K.K.Heppelmann. 1986. Streamwise Distribution of the Recovery Factor and the Local Heat Transfer Coefficient to an Impinging Circular Air Jet. Int. Journal of Heat and Mass Transfer. Vol.29. pp.1227-1235.
4. Camci, C. 2000. Implementation of "*the Invariant h*" method in Liquid Crystal Thermometry Based Heat Transfer Research Including Film Cooling. Proceedings of the Int. Center for Heat and Mas Transfer, Turbine-2000 Symposium, held in Cesme, Izmir, Turkey.
5. Camci, C., K.Kim, S.A. Hippensteele and P.E.Poinsatte. 1993. Evaluation of a Hue Capturing Based Transient Liquid Crystal Method for High Resolution Mapping of Convective Heat Transfer on Curved Surfaces. ASME Journal of Heat Transfer. Vol.115, Number 2. pp. 311-318.
6. Jones,T.V. and S.A.Hippensteele. 1985. High Resolution Heat Transfer Coefficient Maps Applicable to Compund-curve Surfaces using Liquid Crystals in a Transient Wind Tunnel. Developments in Experimental Techniques in Heat Transfer and Combustion. ASME HTD, Vol.71.
7. Ireland, P.T. & T.V. Jones. 1987. The Measurement of Local Heat Transfer Coefficients in Blade Cooling Geometries. AGARD Conference Proceedings on Heat Transfer and Cooling. CP-390, Paper-28.Bergen.Norway.
8. Metzger,D.E, R.S.Bunker and G.Bosch. 1991. Transient Liquid Crystal Measurement of Local Heat Transfer on a Rotating Disk with Jet Impingement. ASME Journal of Turbomachinery. Vol.113. pp. 52-59.
9. Vedula,R.J. and D.E. Metzger. 1991. A Method for the Simultaneous Determination of Local Effectiveness and Heat Transfer Distributions in Three-temperature Convective Situations. ASME paper 91-GT-345.
10. Ekkad, S.V. and J.C.Han. 1996. Heat Transfer Inside and Downstream of Cavities Using a Transient Liquid Crystal Method. AIAA Journal of Thermophysics and Heat Transfer. Vol.10, No.3. pp.511-516.
11. Drost,U., A.Hoffs and A.Bolcs. 1997. Utilization of the Transient Liquid Crystal Technique for Film Cooling Effectiveness and Heat Transfer Investigations on a Flat Plate and a Turbine Airfoil. ASME paper. ASME Gas Turbine Conference. Orlando,Florida.
12. Schultz, D.L. and T.V.Jones. 1973. Heat Transfer Measurements in Short Duration Hypersonic Facilities. AGARDograph 165. London.
13. Oldfield, M.L.G., T.V.Jones, D.L.Schultz. 1978. On-line Computer for Transient Turbine Cascade Instrumentation. IEEE Transactions on Aerospace and Electronic Systems, Vol.AES-14,No.5. pp. 738-749.
14. Jones, T.V. and D.L.Schultz. 1978. Measurement of Heat Transfer Rate to Turbine Blades and Nozzle Guide Vanes in a Transient Cascade. EC-12. 6 th International Heat Transfer Conference.Toronto.pp.73-78.

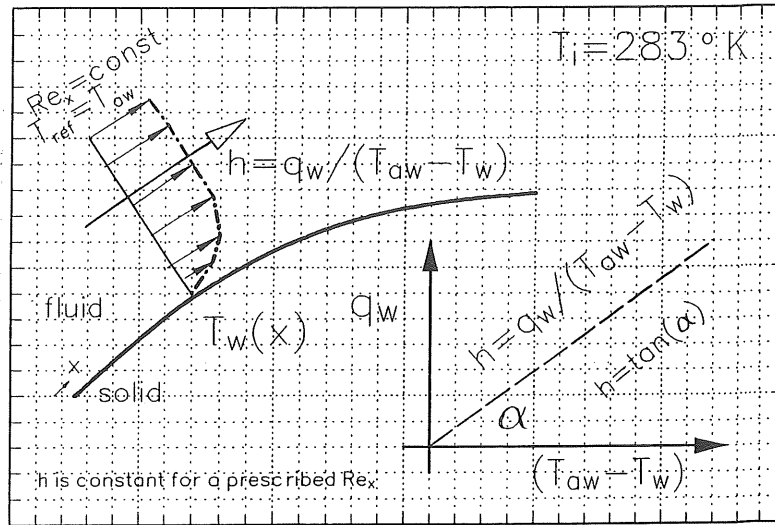


Figure 1 Generic test case definition and nomenclature

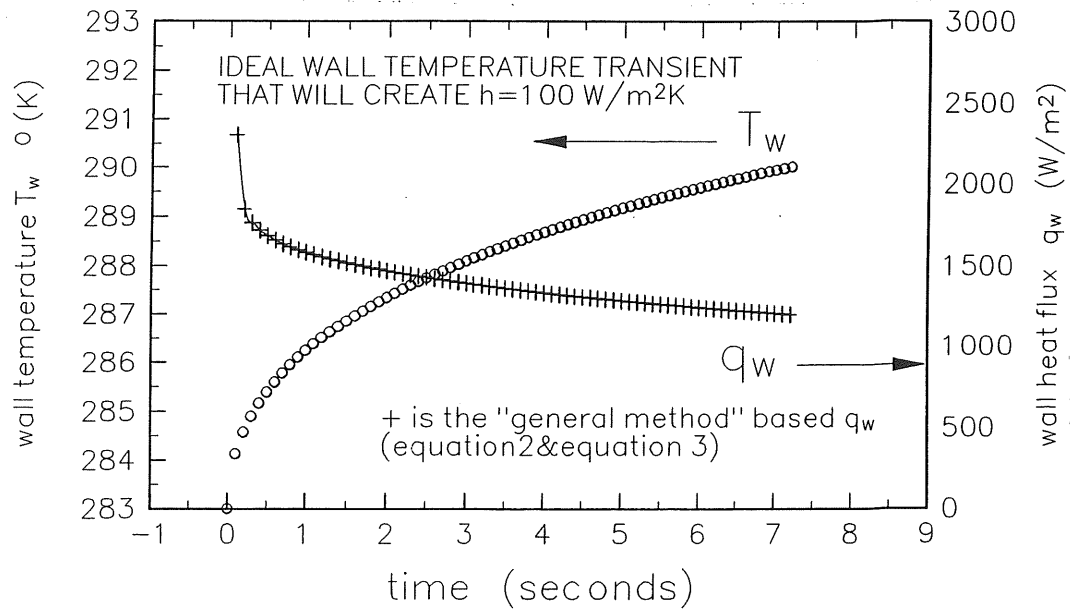


Figure 2 Wall temperature transient recorded at a specific point on heat transfer surface and its corresponding converted wall heat flux trace evaluated from the "general method" (equation 2),  $T_{\infty} = T_{ref} = T_{aw} = 302 \text{ °K}$ ,  $T_i = 283 \text{ °K}$

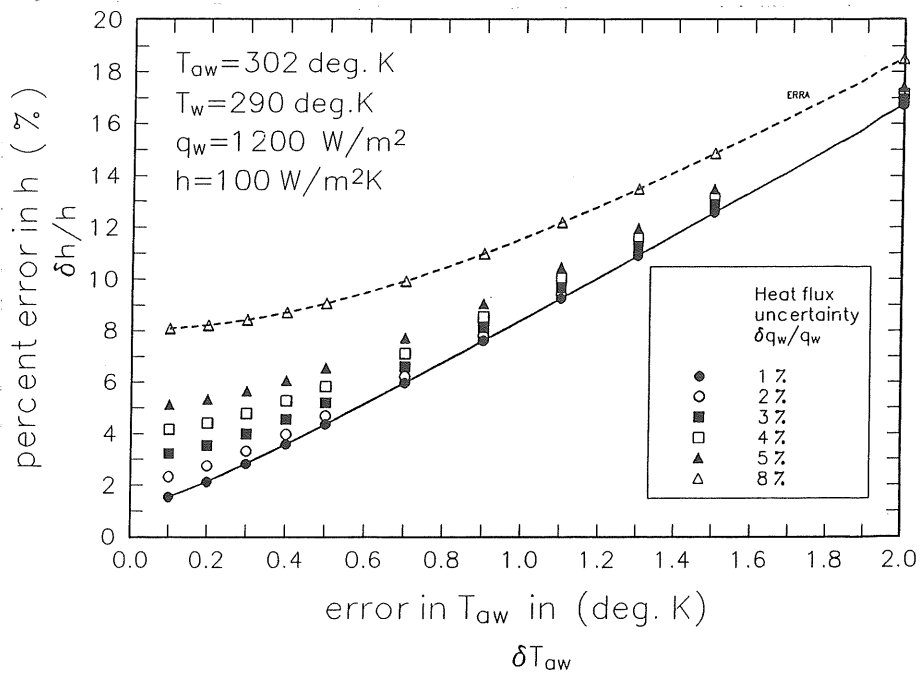


Figure 3 Uncertainty of heat transfer coefficient  $\delta h/h$  for  $\delta T_w = \pm 0.1$  ° K (excellent wall temperature measurement capability)

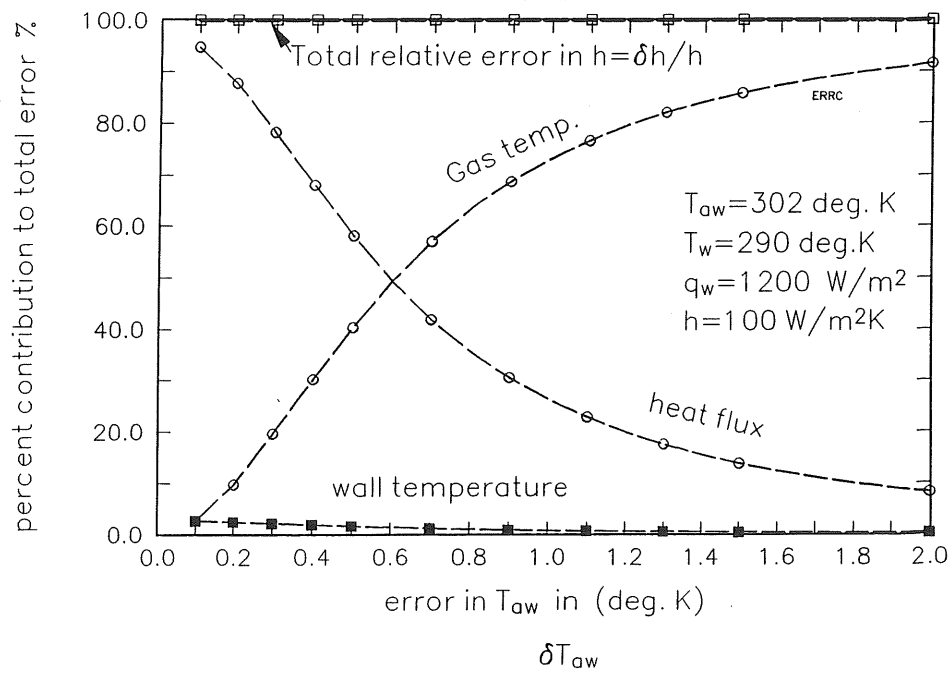


Figure 4 Contribution of individual errors to  $\delta h/h$  (percentage of error norms)

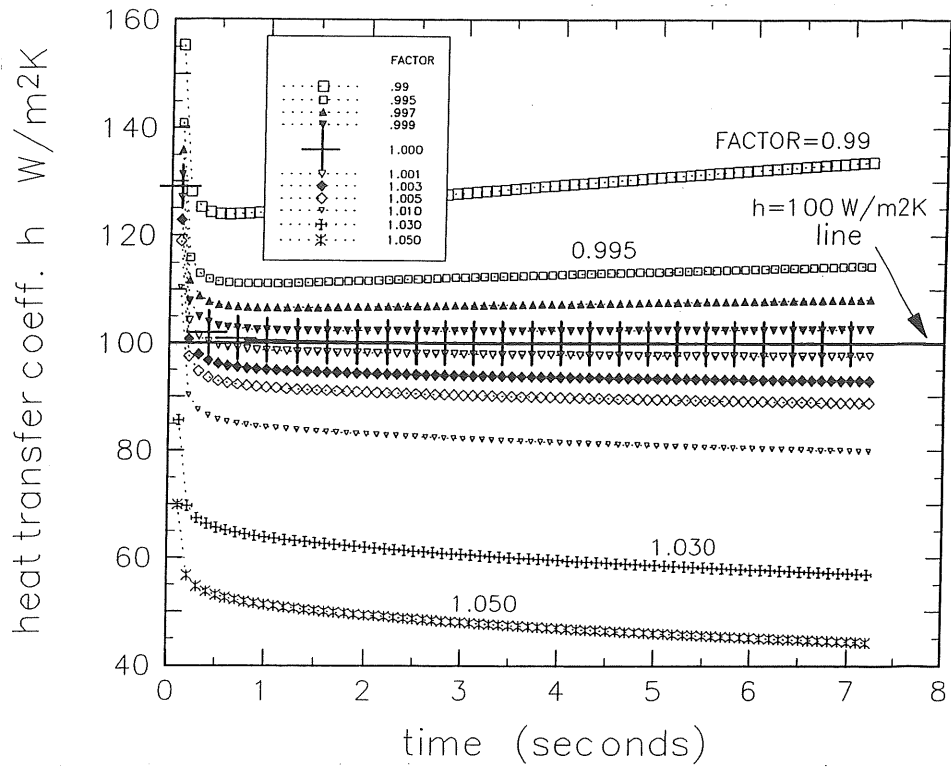


Figure 5 Influence of suggested (iteratively altered) free stream temperature  $[FACTOR * T_{\infty}]$  on heat transfer coefficient  $h$

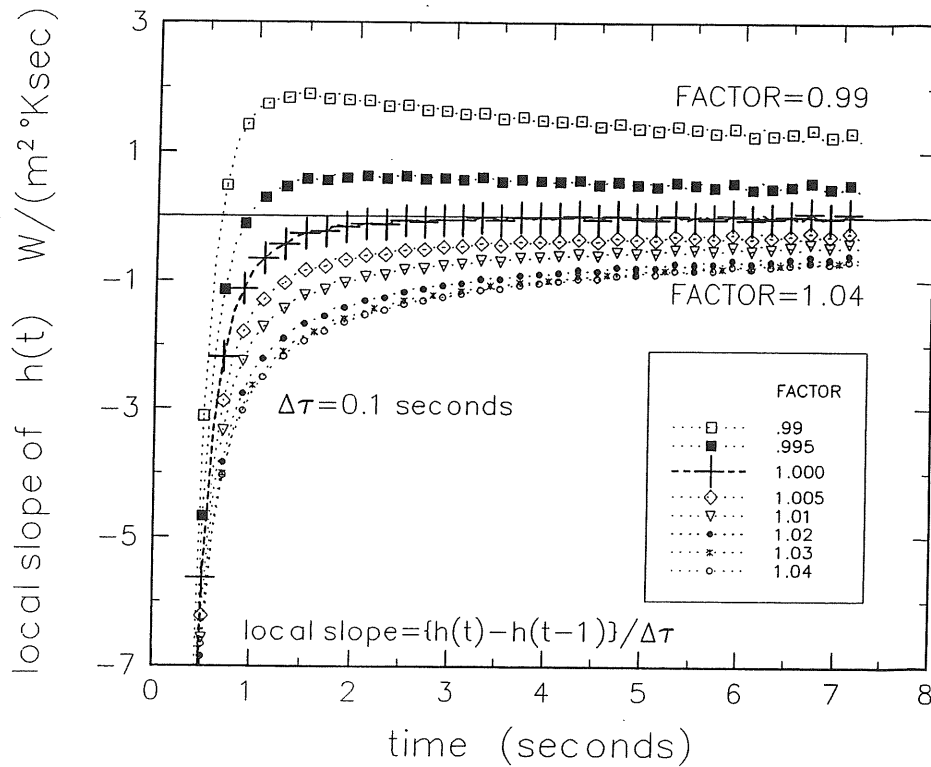


Figure 6 Local slope of heat transfer coefficient  $h$

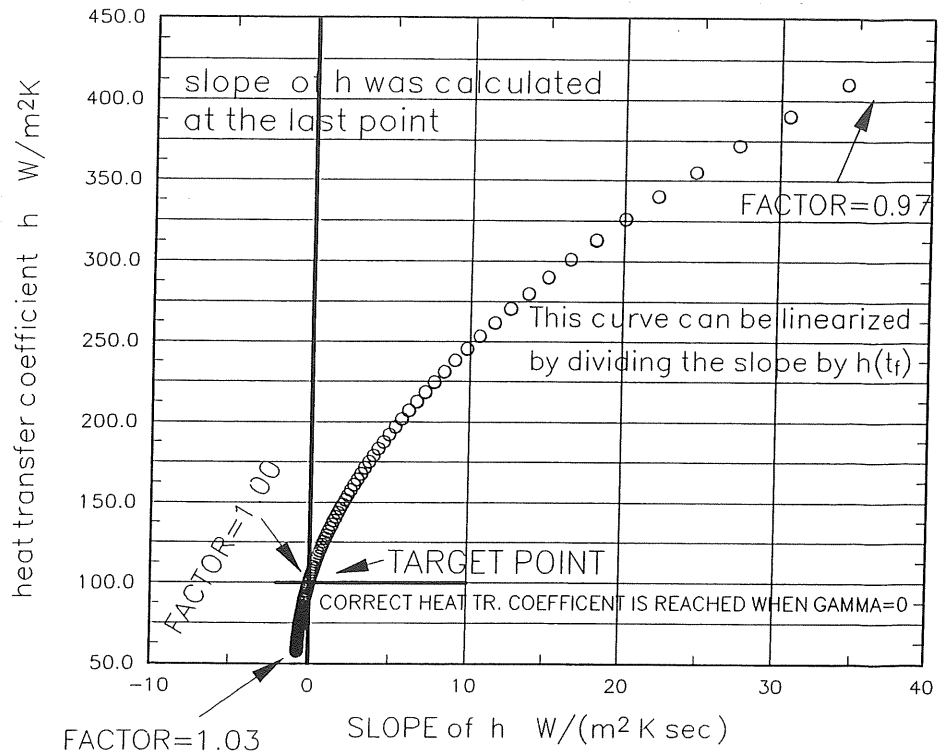


Figure 7 Relationship between "resulting  $h$ " and its timewise slope at the end of the transient run  $t=t_f$

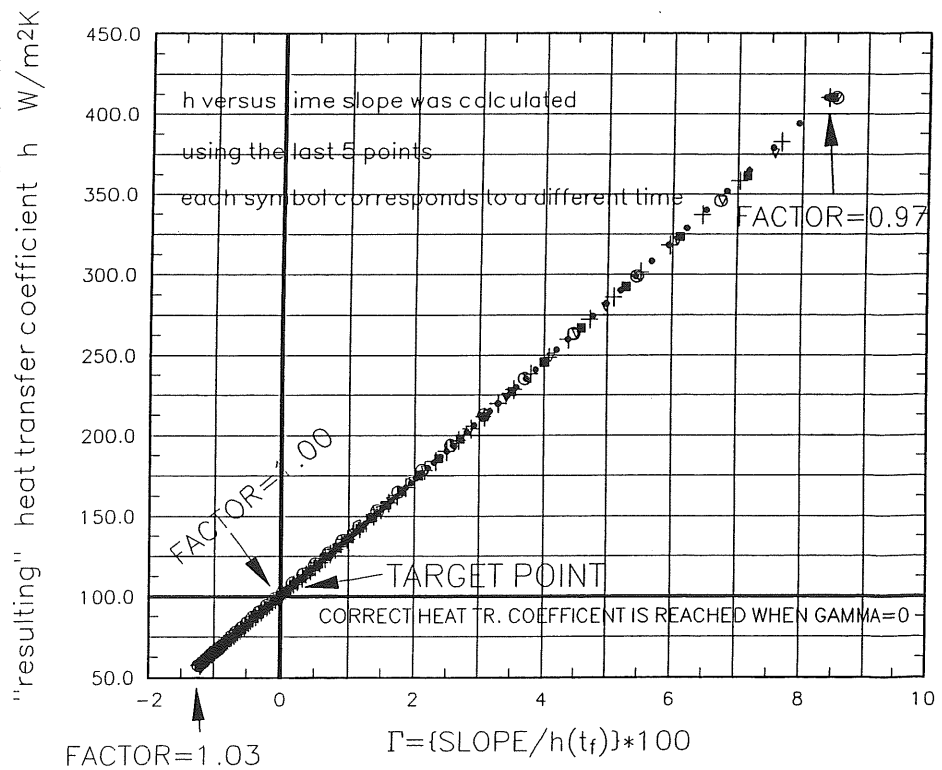


Figure 8 Linearized curve for  $h$  versus timewise slope variation

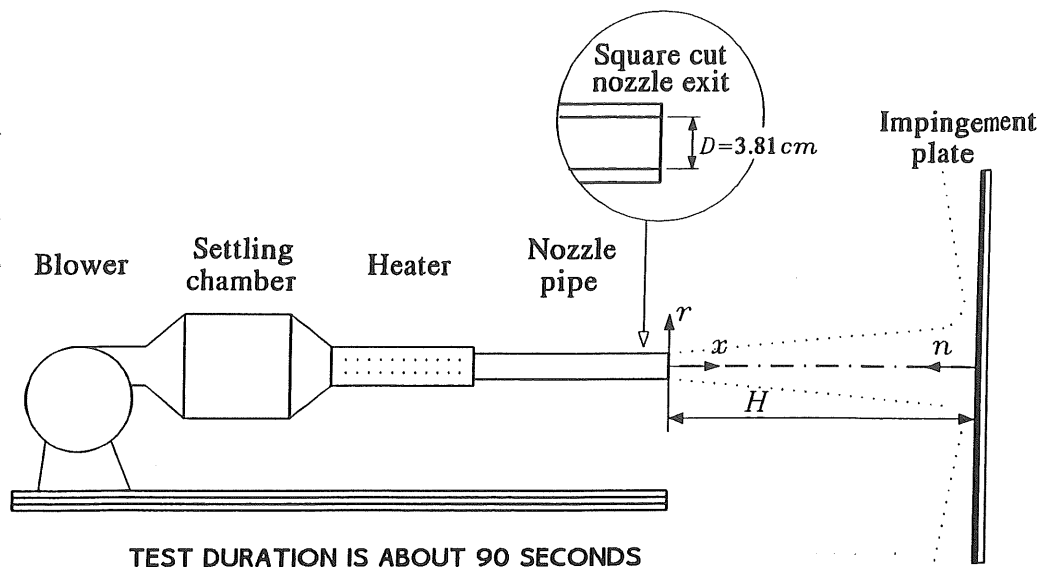


Figure 9 Experimental Confirmation of the "invariant h" method, heated impinging jet details

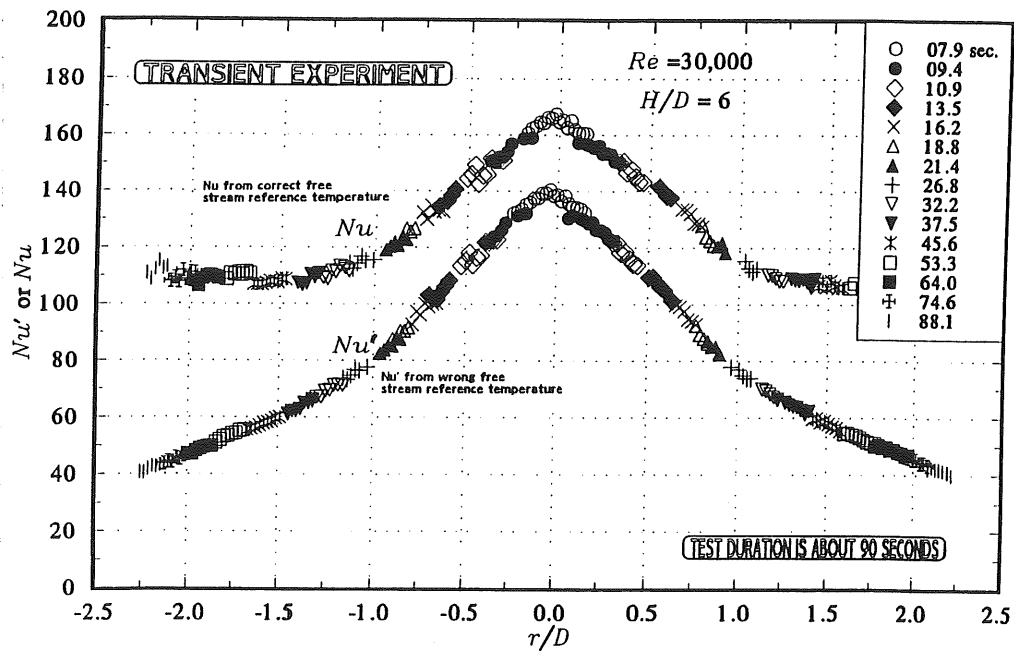


Figure 10 Experimental confirmation of the "invariant h" method, Nu number distribution obtained from the correct free stream reference temperature and Nu' distribution resulting from  $T_{jmax} = 333^\circ \text{ K}$  at the exit of the nozzle, ( $T_i = 296^\circ \text{ K}$ )