Resonator S11, complex plane: VNA calibration vs. switch, before calibration

Raw S_{21} through circulator, switch and cable; no correction except its 22.4 ns cable delay removed. 535-562 MHz shown.
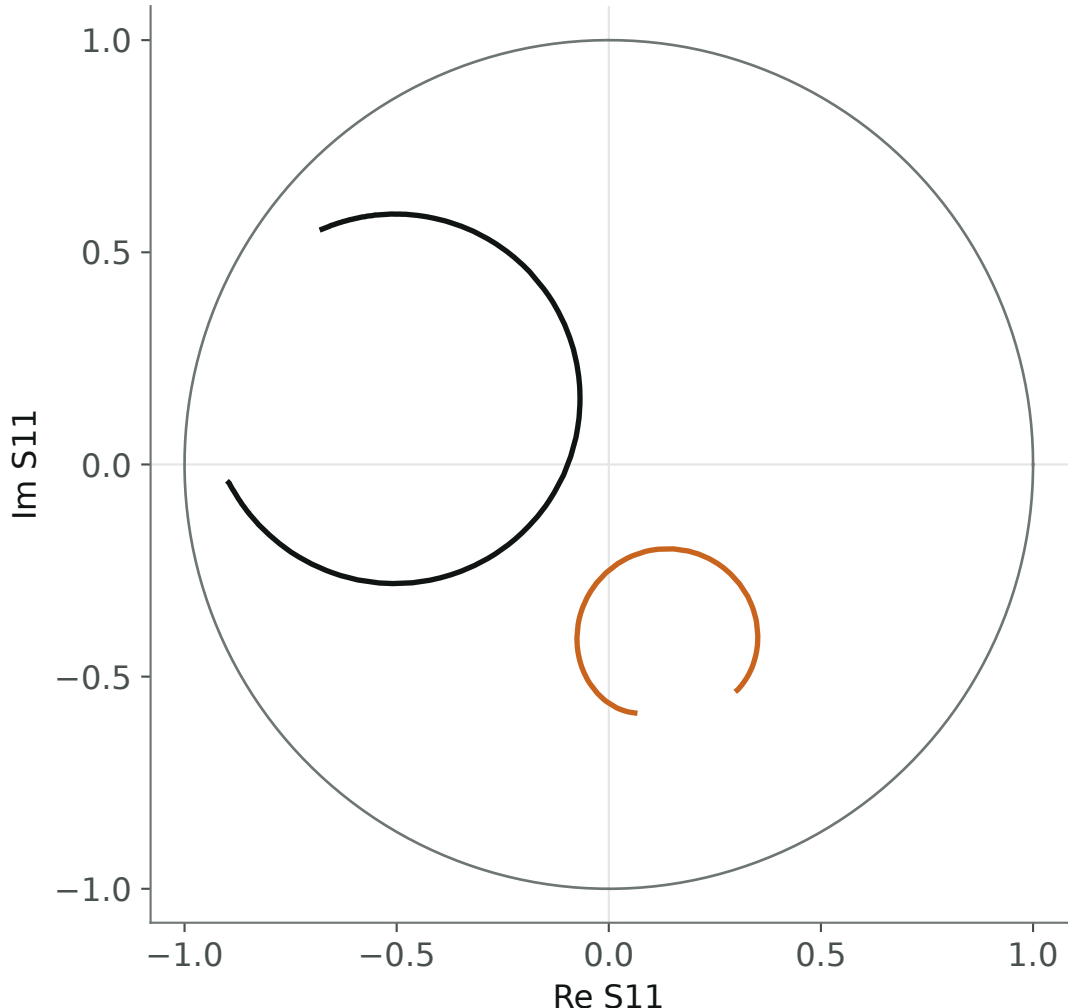
	f_0 (MHz)	Q_i	Q_e	β
—— Resonator alone, VNA cal	548.90	72.6 ± 0.3	87.1 ± 0.1	0.83
—— Via switch, raw	549.40	77.8 ± 1.3	157.2 ± 3.0	0.49