

Ergonomics Evaluation Report

Posture Analysis

- Neck Flexion: Red
- Shoulder Elevation: Green
- Elbow Angle: Red
- Wrist Deviation: Yellow
- Pelvic Tilt: Red

Workstation Analysis

- Chair: SeatDepth: Green

Pain & Risk Summary

Average Pain Level: 7


Main Pain Region(s): Neck, Elbows/Forearms, Hips/Glutes (VAS 8)

Posture & Ergonomic Corrections

- Raise monitor by 18 cm: Increase monitor height by 18 cm so the top edge is at or just below eye level. This will reduce neck flexion from 65° to the ISO-recommended 0–20° range.
- Lower chair seat by 6 cm: Adjust chair height down by 6 cm to bring elbows closer to a 90–110° angle, reducing excessive elbow extension (currently 155°).
- Tilt pelvis upright to 0°: Sit with hips and pelvis upright (0° tilt), ensuring your lower back is supported and your torso is not slouched forward (current tilt: 64°).
- Straighten wrists to neutral (0°): Adjust hand and forearm position so wrists remain straight (0° deviation), minimizing strain and risk of carpal tunnel.
- Raise monitor by 18 cm: Use a monitor riser or stack to elevate your screen by 18 cm, aligning the top with your eye level per ISO 9241-5.
- Lower chair seat by 6 cm: Reduce chair height by 6 cm to achieve proper elbow angle and allow forearms to rest parallel to the desk.
- Add lumbar support cushion (10 cm): Place a 10 cm thick lumbar cushion at your lower back to maintain upright pelvic posture and reduce slouching.

Final Advice

Your pain intensity and posture risks are severe. Please consult a healthcare professional immediately for assessment and management. Ergonomic corrections are critical, but medical evaluation is required. When performing any posture exercises, stop immediately if you experience pain, tingling, or numbness.

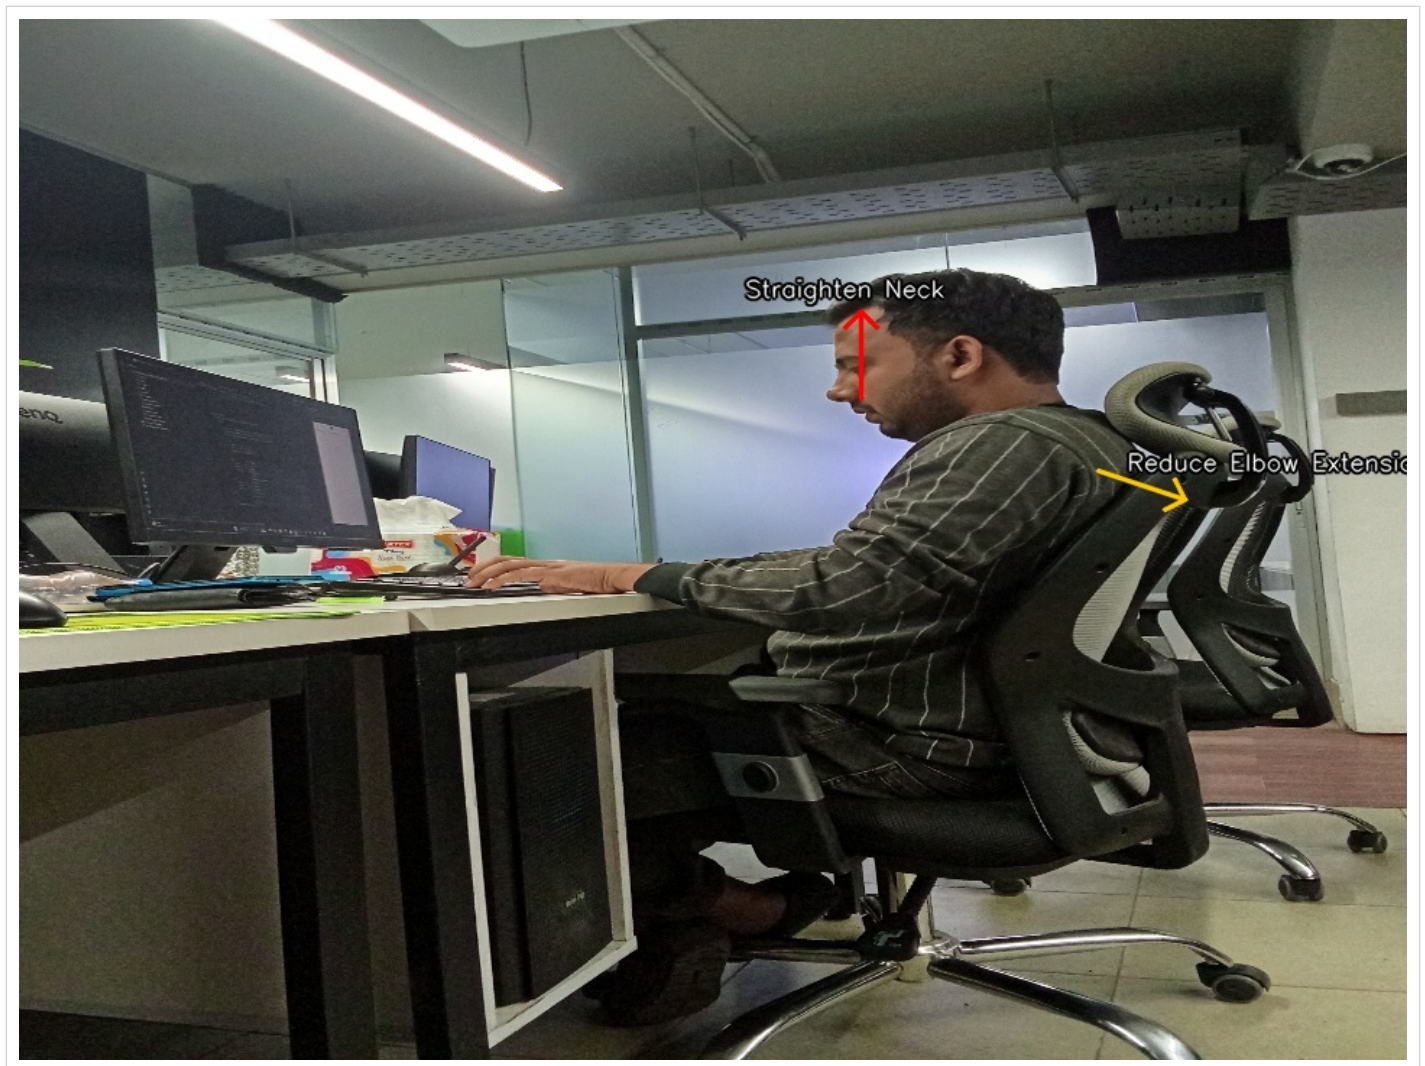

Annotated posture analysis from your uploaded photo