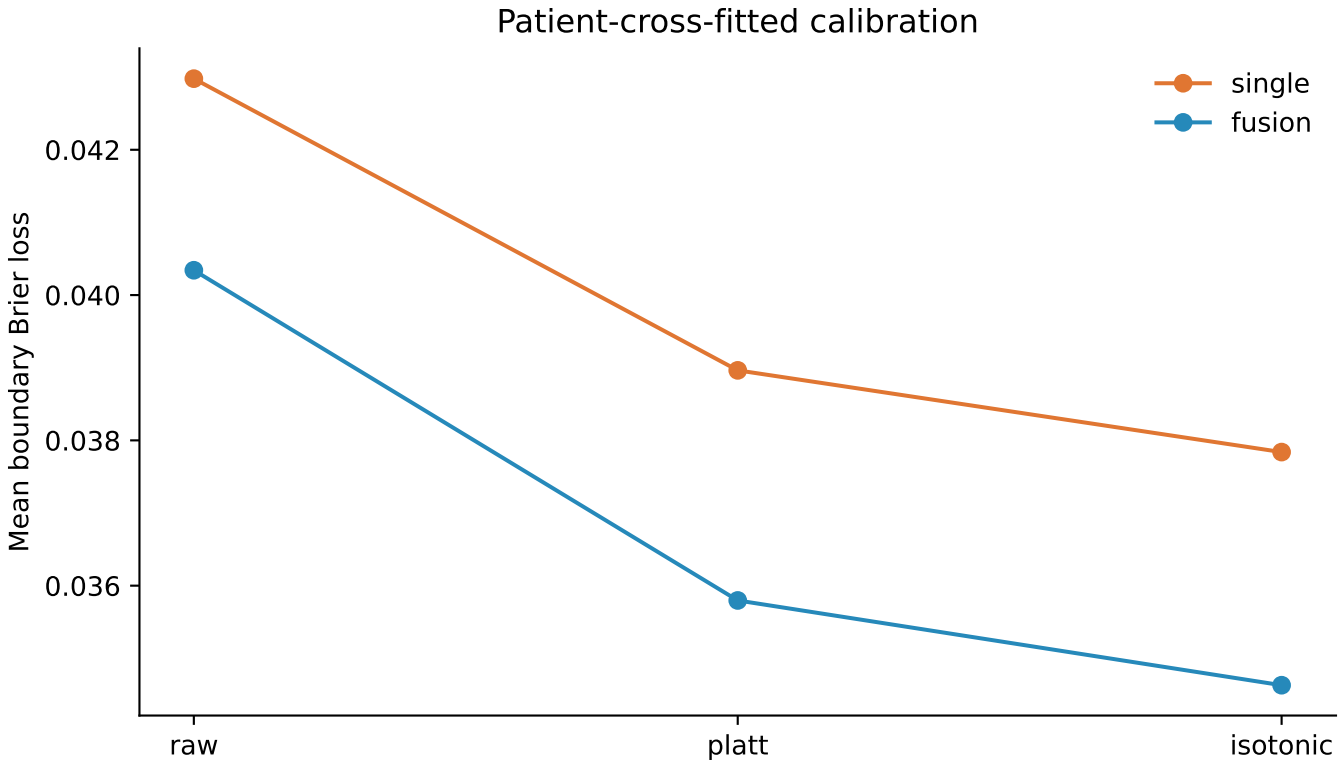
Patient-cross-fitted calibration
single
fusion
Mean boundary Brier loss
0.042
0.040
0.038
0.036
raw
platt
isotonic