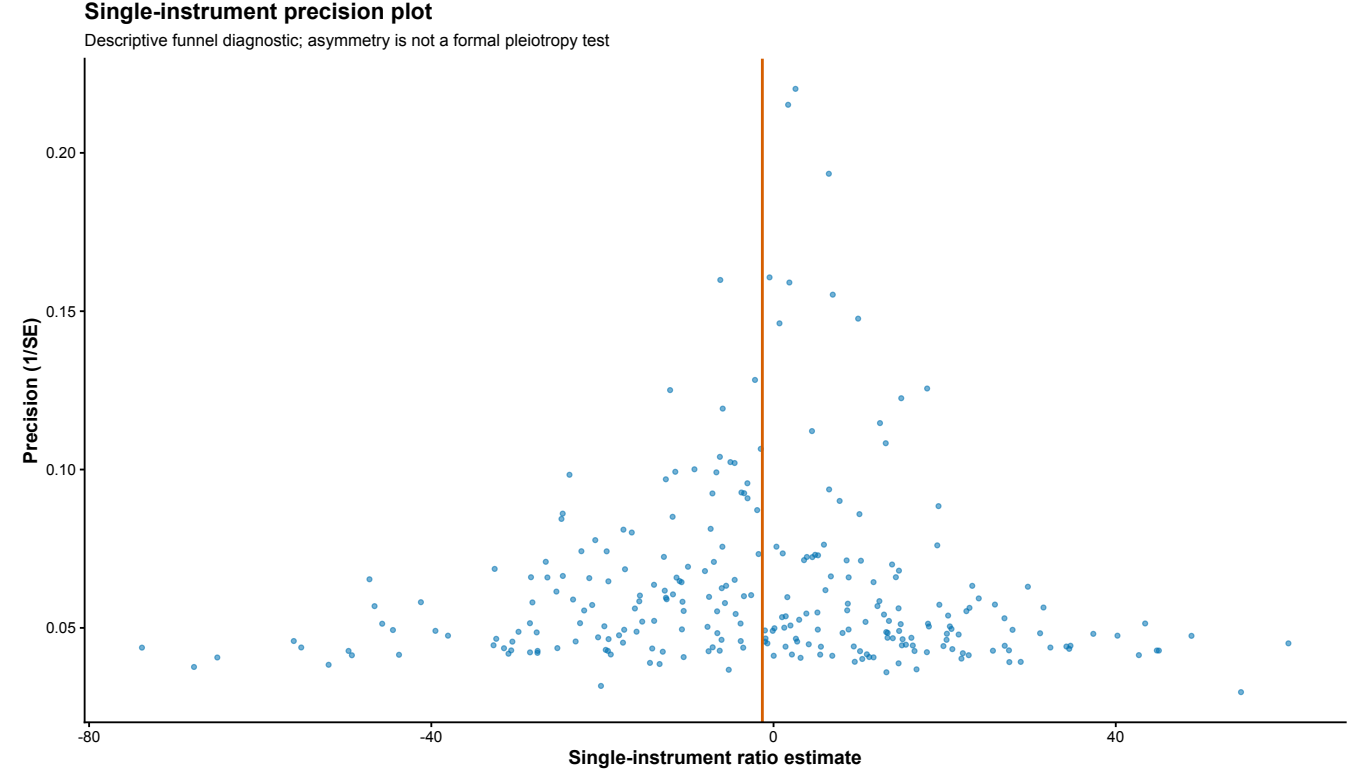
C


Single-instrument precision plot
Descriptive funnel diagnostic; asymmetry is not a formal pleiotropy test
Precision (1/SE)
0.20
0.15
0.10
0.05
-80
-40
0
40
Single-instrument ratio estimate