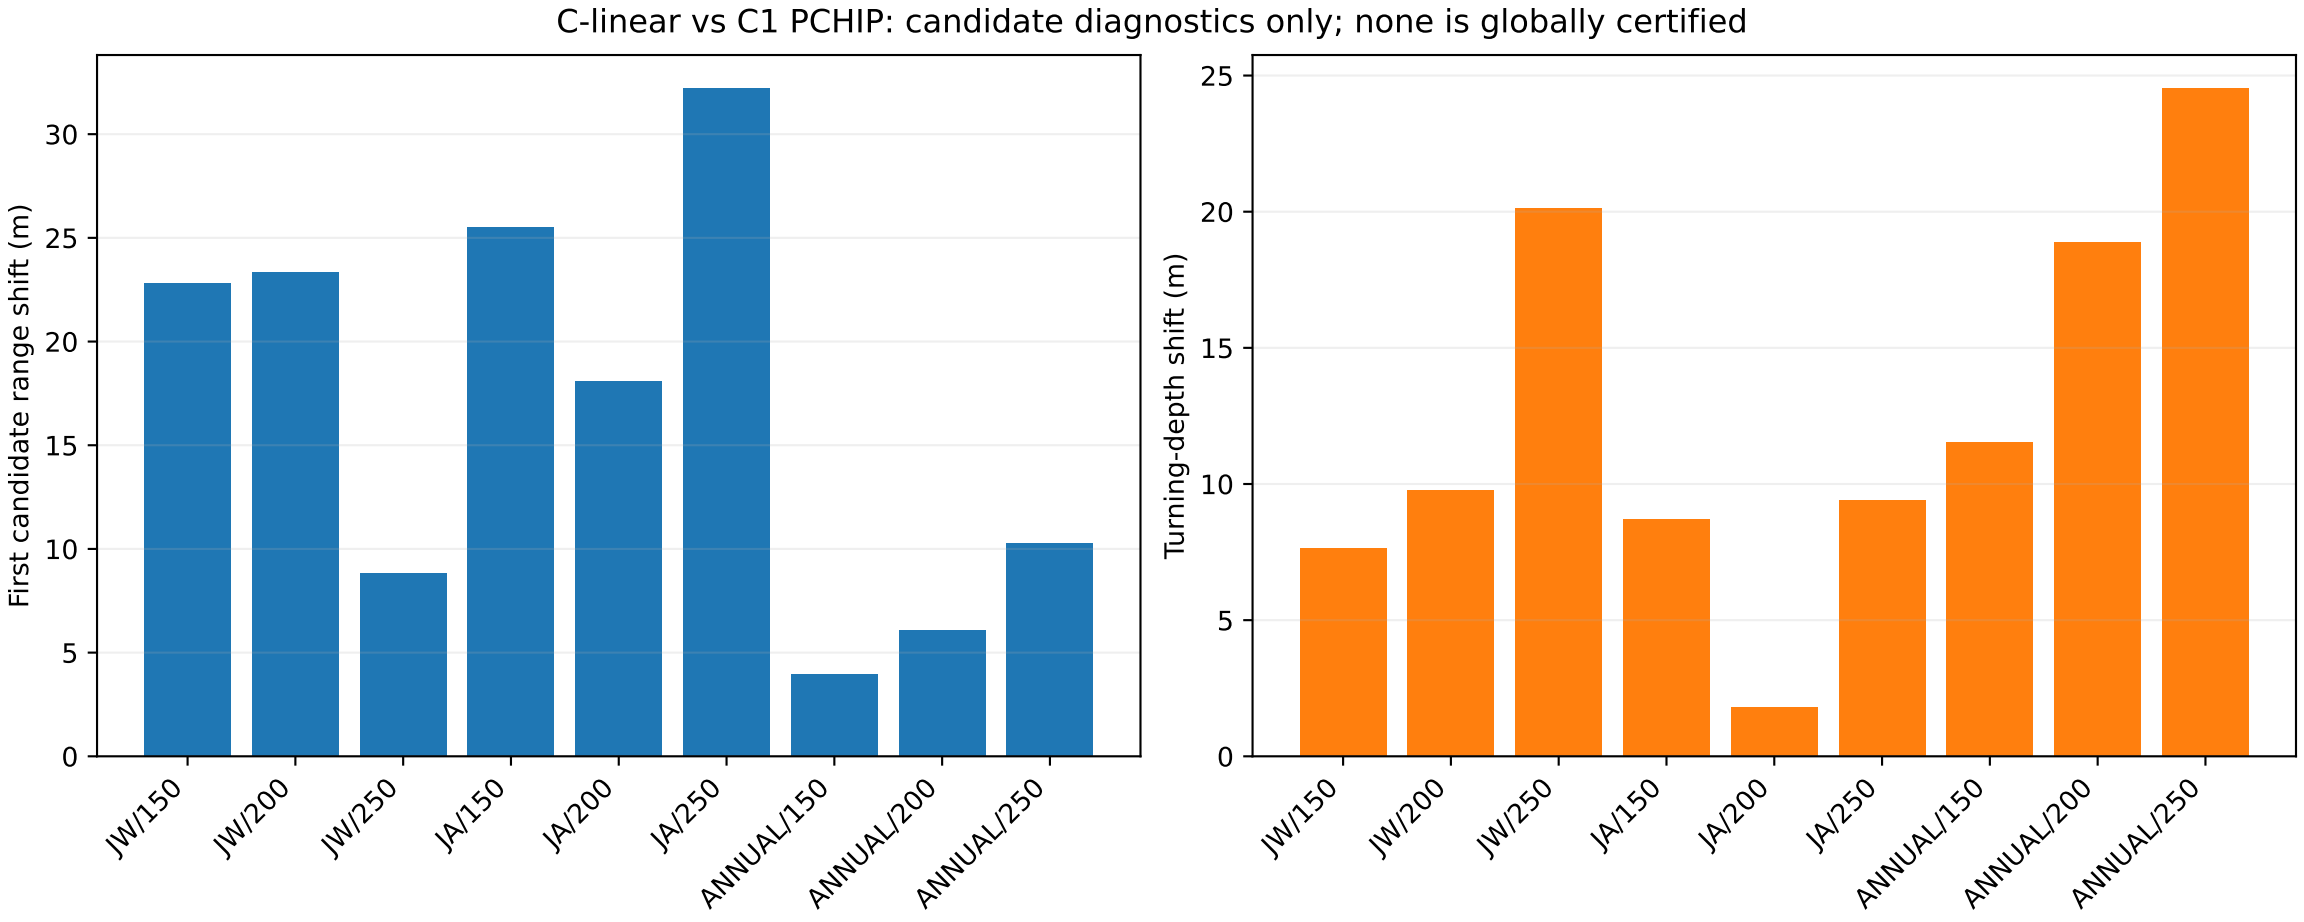
C-linear vs C1 PCHIP: candidate diagnostics only; none is globally certified
First candidate range shift (m)
Turning-depth shift (m)
0
5
10
15
20
25
30
JW/150
JW/200
JW/250
JA/150
JA/200
JA/250
ANNUAL/150
ANNUAL/200
ANNUAL/250