



Regulatory Pathways for Clinical Humanoid Robots: FDA (US) vs. EU MDR + AI Act

**United States
— FDA Pathway**

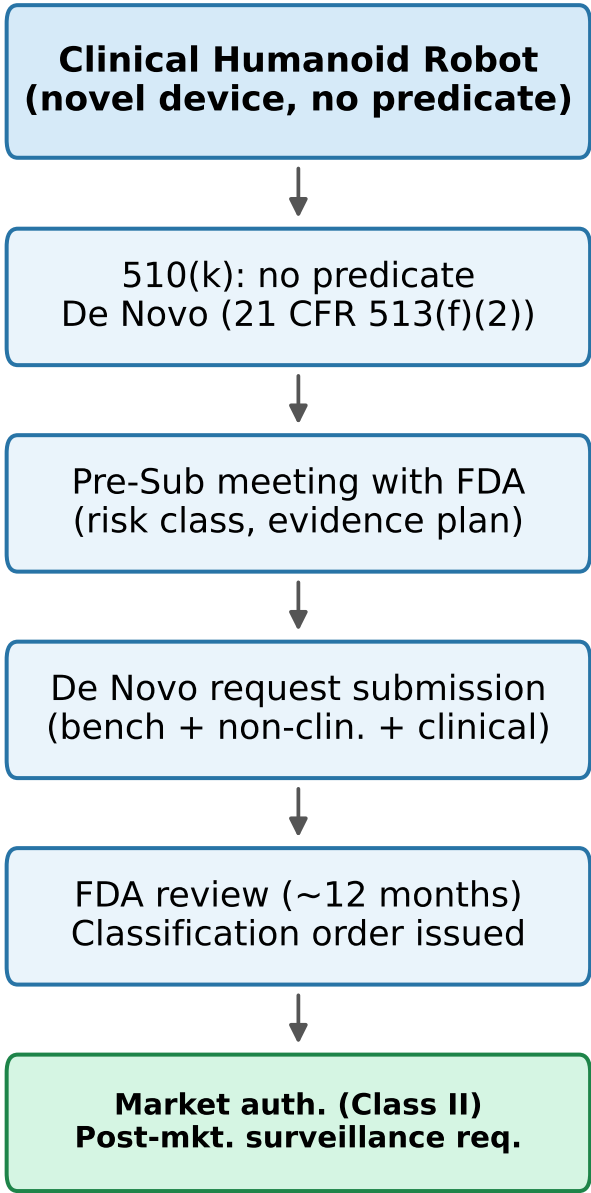

**European Union
— MDR + AI Act**

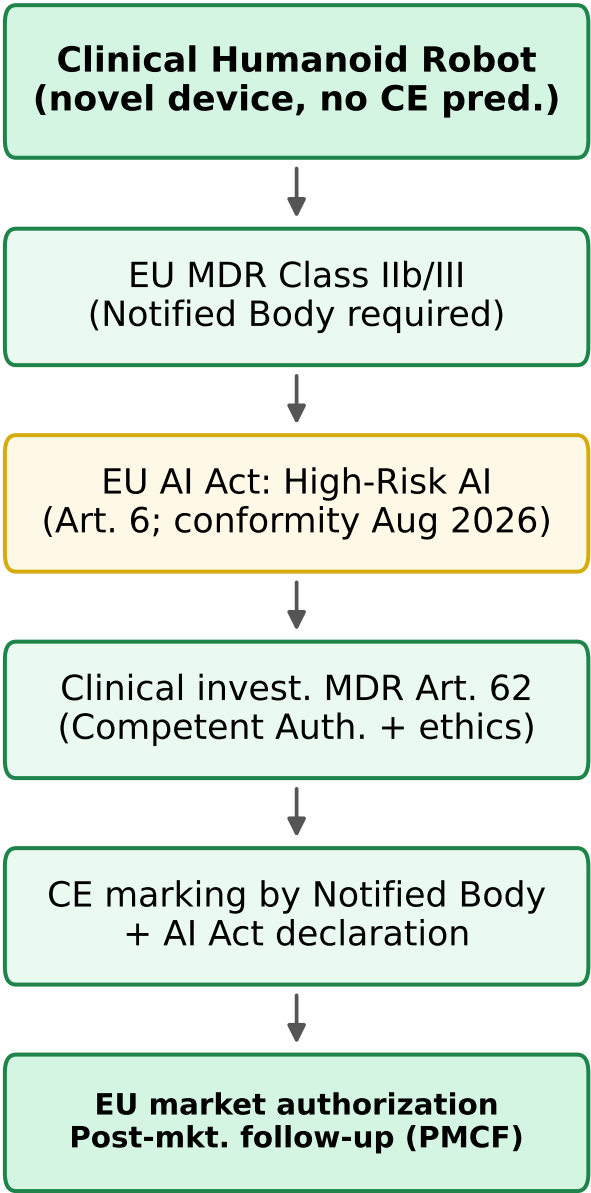

Critical gap (both tracks): no safety standard for
bipedal gait in patient-proximate environments
(ISO 13482 excl. medical devices; ISO/TS 15066: fixed-base arms)