



US FDA

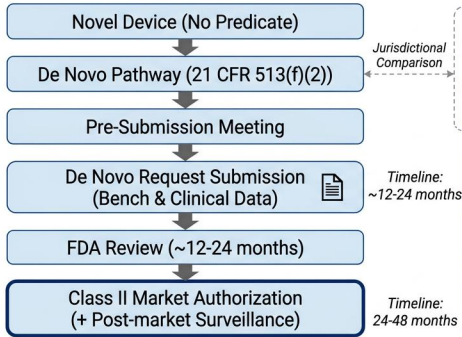

EU MDR & AI Act

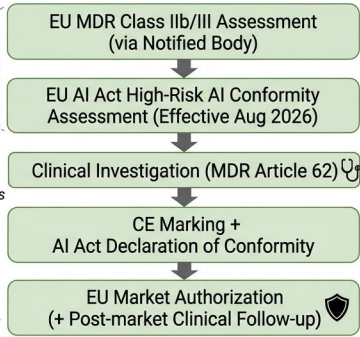

CRITICAL GAP: No accepted safety standard exists for bipedal gait in patient-proximate environments.

ISO 13482: Excludes Medical Devices

ISO/TS 15066: Designed for fixed-base collaborative arms only.