


Regulatory Pathways for Clinical Humanoid Robots: FDA (US) vs. EU MDR + AI Act

United States / FDA Pathway European Union / MDR + AI Act Pathway

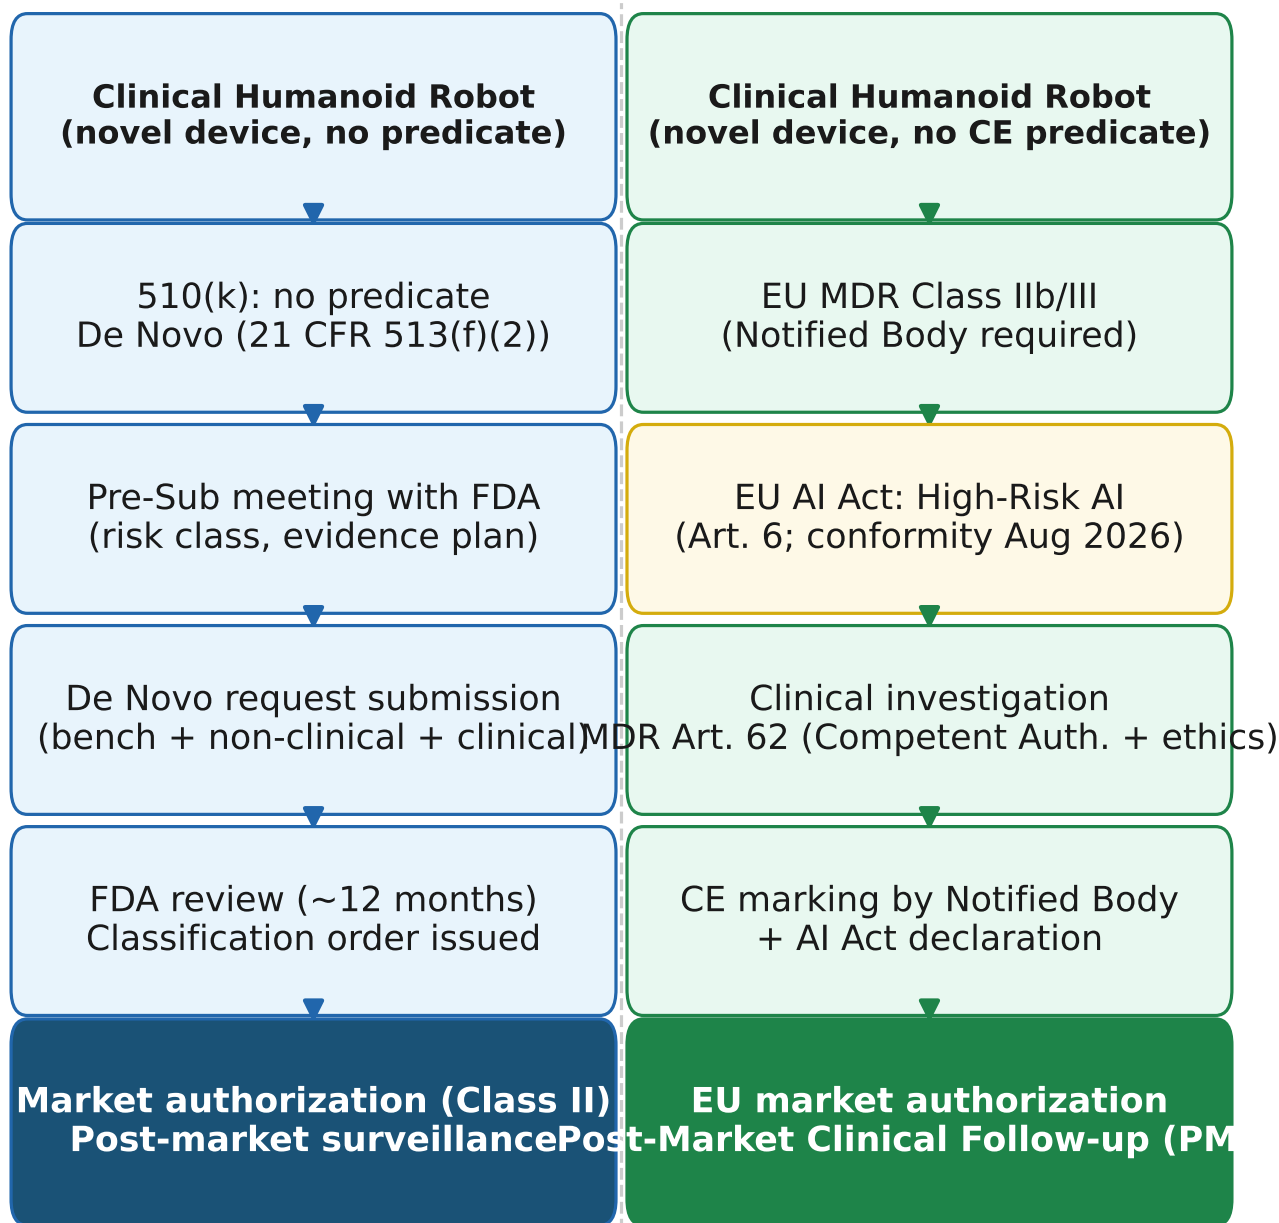

Critical gap (both tracks): no safety standard for
bipedal gait in patient-proximate environments
(ISO 13482 excludes medical devices; ISO/TS 15066: fixed-base arms)