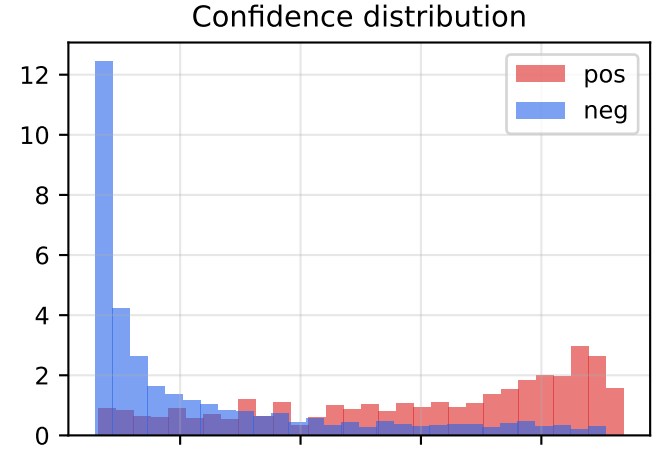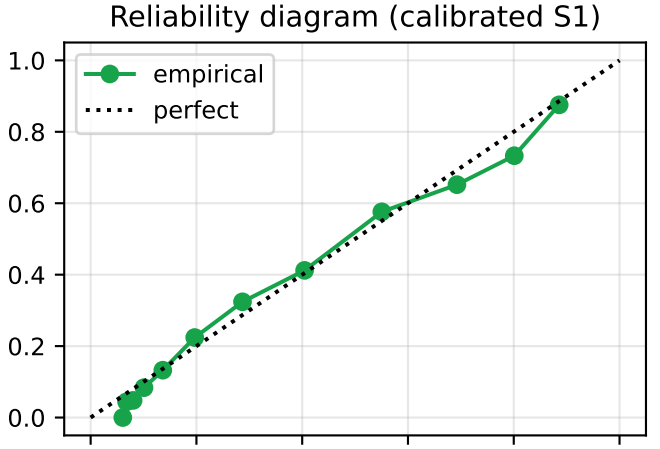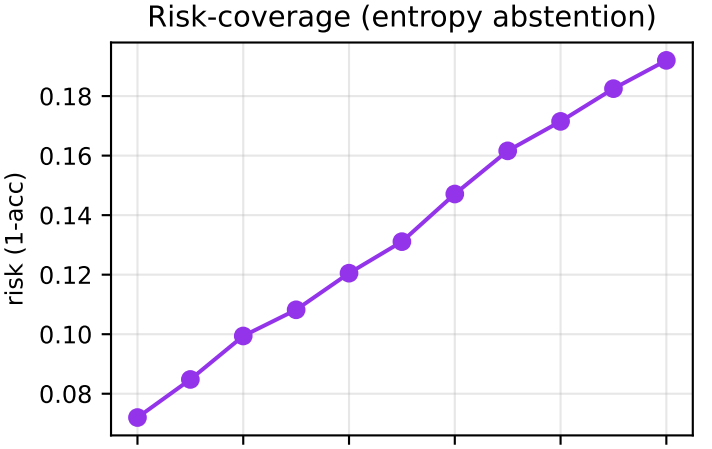Figure 9 — uncertainty and calibration analysis