

# GoodTrade software manual

### Overview

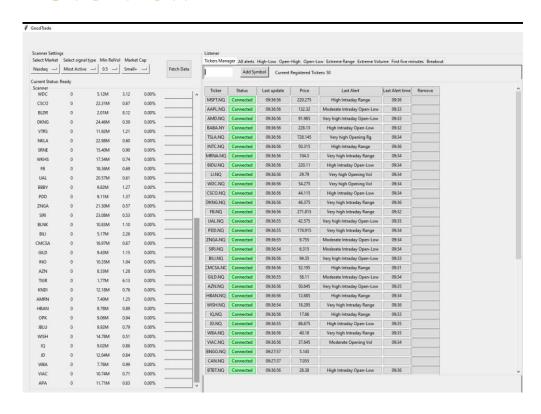

- GoodTrade has two main components: Scanner and Alerts system.
- Scanner filters out live stocks based on certain conditions such as relative volume, most active, etc.
- · Alerts system is able to receive notification when a certain condition is met.
- Symbols showed in Scanner can be added to Alerts system directly and subscribe to all alerts.
- Running requirements:
   Python3.8 or above installed
   Git installed.
- Note: To enable the alert system working, user must be logging onto Ppro TMS for the moment. Future updates will levitate this requirement.

## Alert system - managing symbols







- There are two ways to add symbols to the alert system; 1. input it directly from the Tickers Manager. 2. Add it from Scanner.
- To remove a symbol from the alerts listener, simply click remove in the Tickers Manager.
- When a symbol is added to the listener, it is automatically subscribed to all alerts.

#### **Bulk Management**

- To edit many symbols more efficiently, user is able to open list.txt and add, or delete symbols.
- Note: User should perform this operation before opening the application.
   Any changes of list.txt during application running will not be saved correctly.






## Alert system - Receiving alert.

The user will receive an alert in three ways:


1. Most recent alert via Tickers manager. Last Alert: the type of alert. Last Alert time: The time the alert was produced.



- 2. Evaluation in alert-condition panel (Extreme Range, etc.)
- 1.56 from mean meaning current value is 1.56 standard deviation above the mean.
- tint indicates the extent of the condition: red: very high (2 std and more), yellow: high(1-2 std range), green: worth noting(0.5-1), and white: normal(mean within 0.5 std)

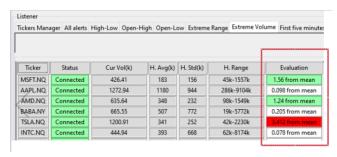

3. All alerts panel displayed each alert received.

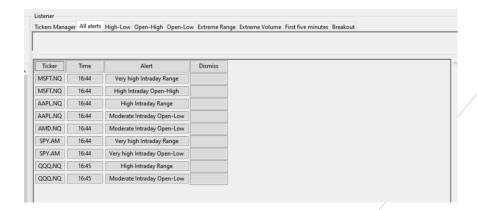

### Alert system - alerts type

ts High-Low Open-High Open-Low Extreme Range Extreme Volume First five minutes Breakout

The alert system supports conditions:

#### · High-Low:

 Evaluate a stock based on its current day range and 10 days historical range.

#### Open-High;

• Evaluate a stock based on its current day open-high and 10 days historical open-high range.

#### · Open-Low:

 Evaluate a stock based on its current day open-low and 10 days open-low historical range.

#### • Extreme Range:

• Evaluate a stock based on its last 5 minutes range and historical average 5 minutes range.

#### Extreme Volume:

 Evaluate a stock based on its last 5 minutes volume and historical average 5 minutes volume.

#### • First five minute:

• Evaluate a stock based on its opening range and volume to its10 days opening average.

#### • Breakout:

 Receive notification when price breaks given support/resistance level.

## Alert system - high low



Cur Range: Current day high-low range.

Cur High: Current day high Cur Low: Current day low

H.Avg: Historical 10 days Average daily range H.Std. Historical 10 days daily range standard

deviation

H.Range. Historical range of daily

## Alert system - open high/ Open Low

Tickers Mana	ger All alerts	High-Low	Open-High	Open-Lov	v Extreme	Range	Extreme Volume	First five minutes	Breakout
Ticker	Status	Cur Range	Cur Open	Cur High	H. Avg	H. Std	H. Range	Evaluation	
			·						_
MSFT.NQ	Connected	5.15	221.7	226.85	3.72	1.251	2.41-6.72	1.143 from mean	
	Connected	0.66	134.08	134.74	3.439	1.128	1.65-4.861	-2.464 from mean	
AAPL.NQ	Connected	0.00							
AAPL.NQ AMD.NQ	Connected	0.54	92.1	92.64	2.441	0.935	1.2-4.2	-2.033 from mean	<u>=</u>

Cur Range: Current day open-high range.

Cur High: Current day high Cur Open: Current day open

H.Avg: Historical Average daily range of Open-High H.Std. Historical daily Open-High standard deviation

H.Range. Historical range of daily Open-High

### Alert system - Extreme range

Tickers Man	ager All alerts	High-Low	Open-High	Open-Low	Extreme Range	Extreme Volume	First five minutes	Breakout
	_	·lr						
Ticker	Status	Cur Range	H. Avg	H. Std	H. Range	Evaluation	1	
AAPL.NQ	Connected	0.045	0.341	0.233	0.06-1.67	-1.27 from m	ean	
AMD.NQ	Connected	0.035	0.263	0.171	0.08-1.37	-1.333 from n	nean	
BABA.NY	Connected	0.125	0.789	0.677	0.13-4.642	-0.981 from n	nean	
TSLA.NQ	Connected	0.585	2.701	1.577	0.54-10.13	-1.342 from n	nean	
BIDU.NQ	Connected	0.06	0.969	0.845	0.088-8.14	-1.076 from n	nean	
BILI.NQ	Connected	0.18	0.49	0.531	0.07-5.7	-0.584 from n	nean	

Cur Range: Current last 5 minutes range

H. Avg: Historical 5 minutes average

H. Std: Historical 5 minutes range standard deviation

H. Range: range on Historical 5 minutes range

## Alert system - Extreme volume

ickers Mana	ger All alerts	High-Low	Open-High	Open-Lo	w Extrem	e Range	Extreme Volu	me First five minute
Ticker	Status	Cur V	ol(k)	l. Avg(k)	H. Std(k)	H.	Range	Evaluation
MSFT.NQ	Connected	426	.41	183	156	451	k-1557k	1.56 from mean
AAPL.NQ	Connected	1272	2.94	1180	944	286	k-9104k	0.098 from mean
AMD.NQ	Connected	635	.64	348	232	981	k-1549k	1.24 from mean
BABA.NY	Connected	665	.55	507	772	191	k-5772k	0.205 from mean
TSLA.NQ	Connected	1200	).91	341	252	421	c-2230k	3.412 from mean
INTC.NQ	Connected	444	.94	393	668	621	c-8174k	0.078 from mean
MRNA.NQ	Connected	412	.95	293	243	401	k-2185k	0.494 from mean
BIDU.NQ	Connected	151	.61	103	146	51	k-996k	0.333 from mean
LI.NQ	Connected	748	.22	196	191	281	k-1509k	2.891 from mean
WDC.NQ	Connected	128	.95	51	71	31	k-644k	1.098 from mean
CSCO.NQ	Connected	259	.61	122	113	281	k-1281k	1.218 from mean
DKNG.NQ	Connected	266	.77	138	112	231	k-1200k	1.15 from mean


Cur Vol: Current last 5 minutes volume. (unit is thousand)

H.Avg: Historical 5 minutes average volume

H.Std: Historical 5 minutes volume standard deviation

H.Range: range on Historical 5 minutes range

## Alert system - First five minutes (opening 9:30-9:35)

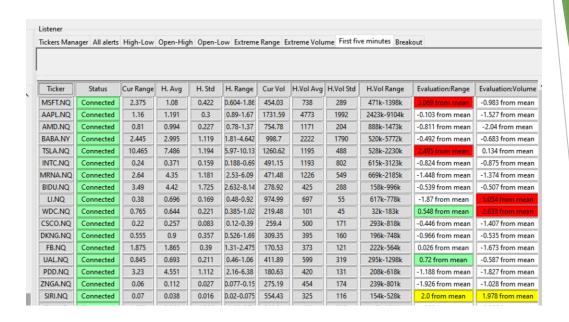

Cur Range/ Cur vol: opening 5 minutes range /vol H.Avg: Past 10 days average opening 5 minutes range/vol

H.Std: Past 10 days opening 5 minutes range/vol standard

deviation

H.Range Past 10 days range on opening 5 minutes range/vol

## Alert system - breakout

Listener								
Tickers Mana	ger All alerts	High-Low	Open-High	Open-Low	Extreme Range	Extreme Volum	e First five minutes	Breakout
Ticker	Status	Support	t Resista	nce Cu	ır Price E	valuation		
	Status		Resista			valuation		
MSFT.NQ	Connected	218	220	2	19.95			
AAPL.NQ	Connected	132	132.5	1	131.8 Sup	oort breakout		
AMD.NQ	Connected	93	94.5	9	4.505 Resist	ance breakout		
BABA.NY	Connected	228	230	2	28.96			
TSLA.NQ	Connected	730	740	73	39.565			
BIDU.NQ	Connected	0.0	0.0	2	225.7			

- Current stage require manually input support/resistance level.
- Upon breaching the level, an alert is generated.
- Future version auto support-resistance recognition will be added.