

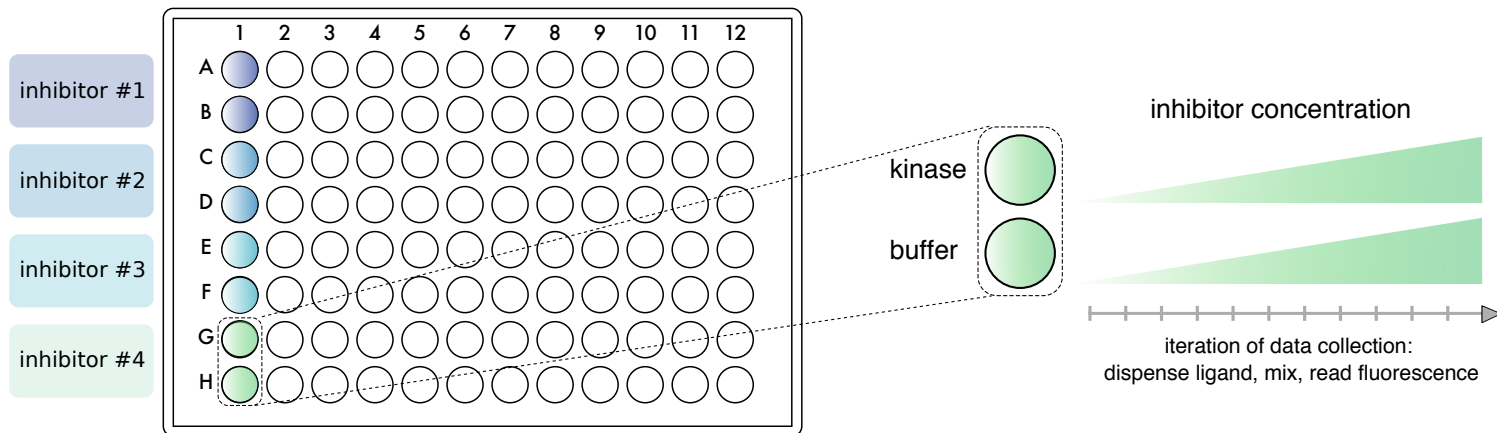
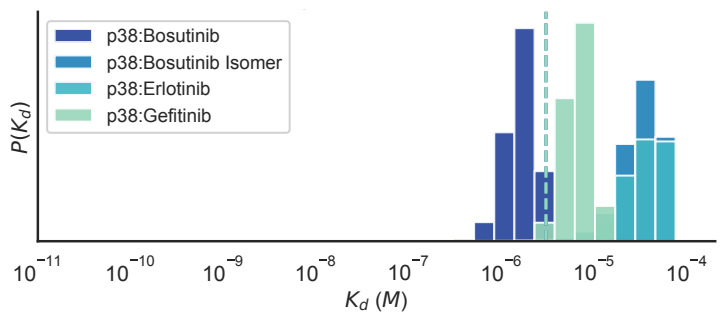


A

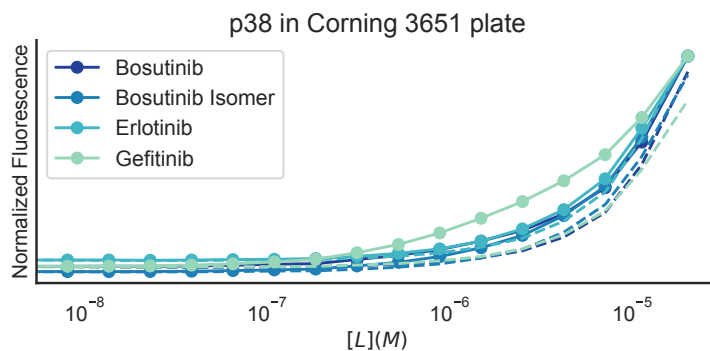

B

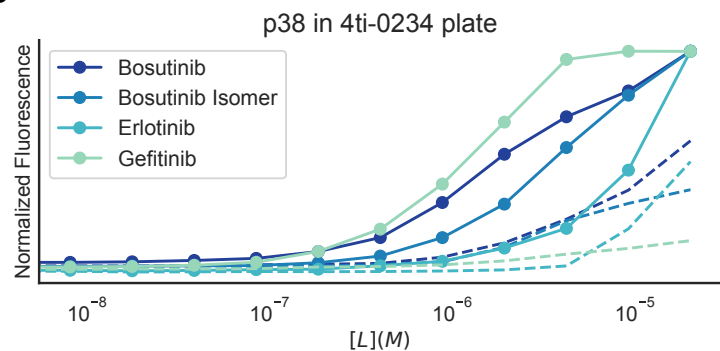

PLACE HOLDER: WILL BE REPLACED  
WITH HISTOGRAM FOR 4 LIGANDS  
WITH CORNING 3651 PLATE