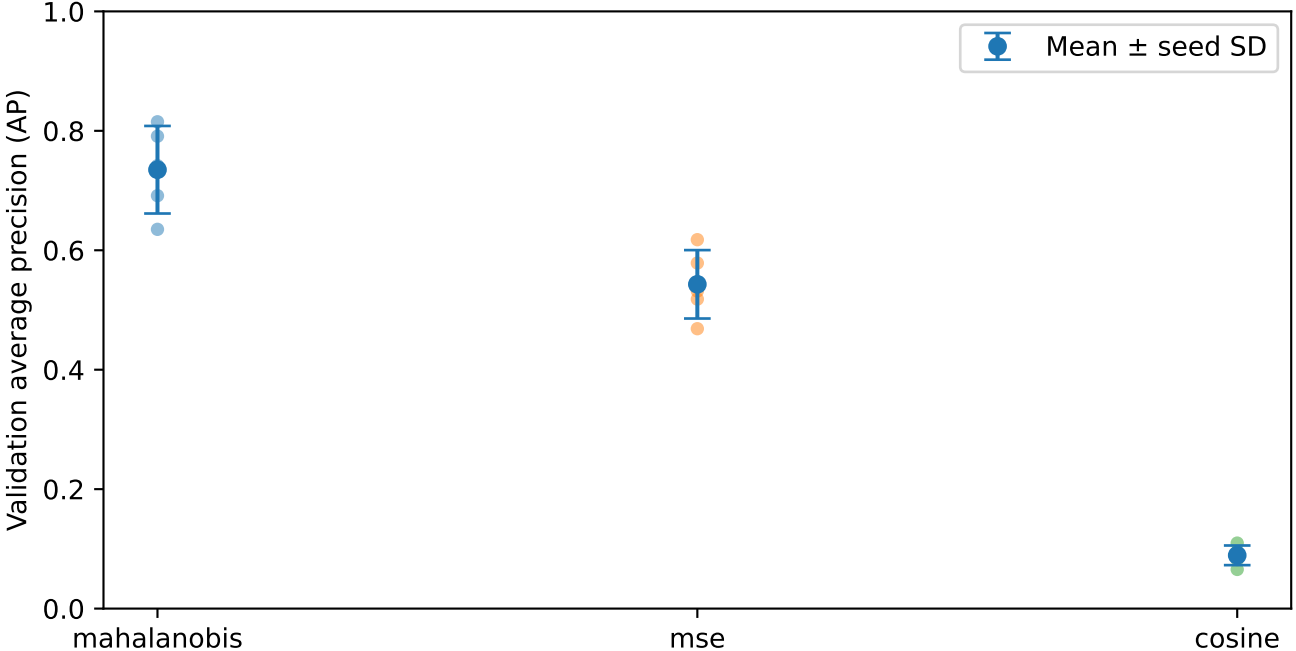
Validation average precision (AP)
1.0
0.8
0.6
0.4
0.2
0.0
Mean ± seed SD
mahalanobis
mse
cosine