


M1 same-channel FDT protocol

Ordinary non-KMS or protocol counterexamples

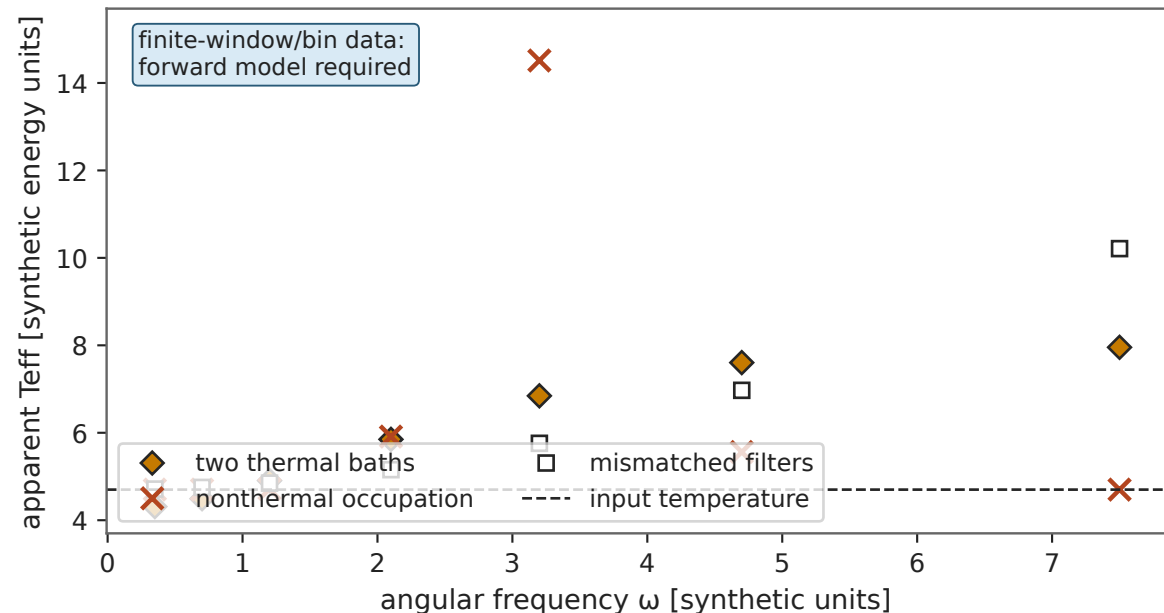

Ordinary non-KMS/protocol counterexamples; mismatch is not by itself ECT evidence.