

Quality Assurance (04-May-2020, 11:40:07, #141814)

Coil Check FlexSmall_4 Success (04-May-2020, 11:40:08 » 04-May-2020, 11:43:47)

Comments (0)

#	Timestamp	Comment
No comments for this function.		

Summary

Summary

	Status
098_FlexSmall_4_Tra	OK
Program Result	Success

Details


Protocol: 098_FlexSmall_4_Tra

Coil Info

Coil ID	Serial Number	Part Number
FlexSmall_4	32023	10185553

Coil: FS1

Signal

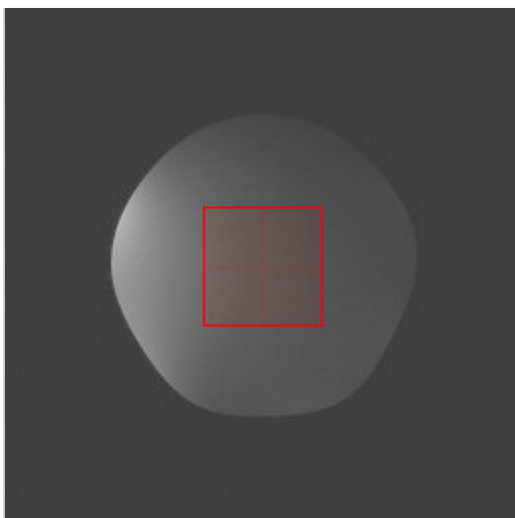

S/N

Parabola Fit	
Value	Min
32.1	24.0

Brightness


Parabola Fit		
Value	Min	Max
320	125	500

Homogeneity and Transmitter Amplitude

Variable	Value	Unit
Transmitter Amplitude	298	V

Coil: FS2

Signal

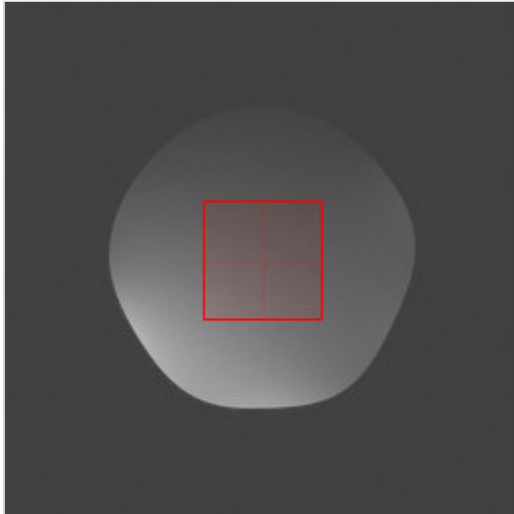

S/N

Parabola Fit	
Value	Min
37.6	24.0

Brightness


Parabola Fit
364

Homogeneity and Transmitter Amplitude

Variable	Value	Unit
Transmitter Amplitude	298	V

Coil: FS3

Signal

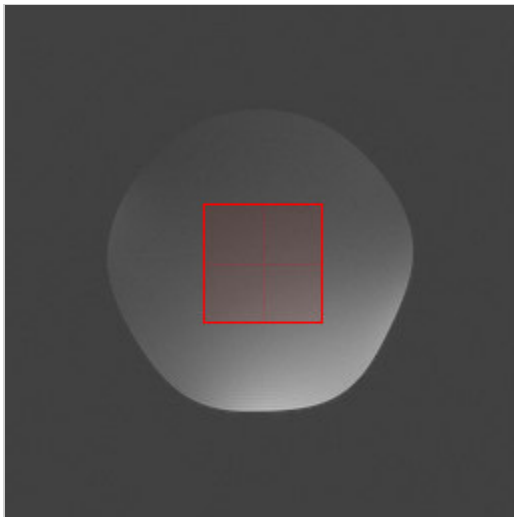

S/N

Parabola Fit	
Value	Min
26.0	23.0

Brightness


Parabola Fit
261

Homogeneity and Transmitter Amplitude

Variable	Value	Unit
Transmitter Amplitude	298	V

Coil: FS4

Signal

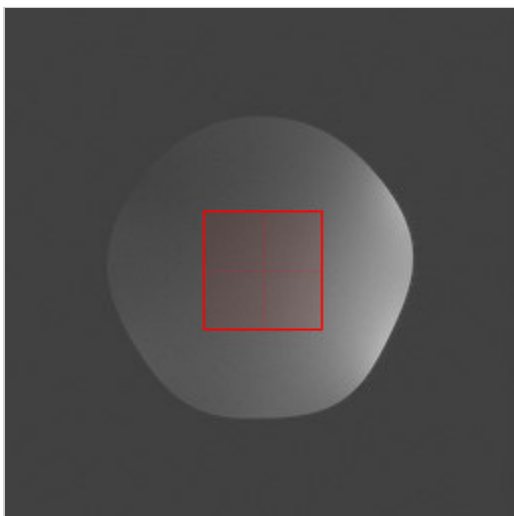

S/N

Parabola Fit	
Value	Min
30.0	23.0

Brightness

Parabola Fit

286

Homogeneity and Transmitter Amplitude

Variable	Value	Unit
Transmitter Amplitude	298	V