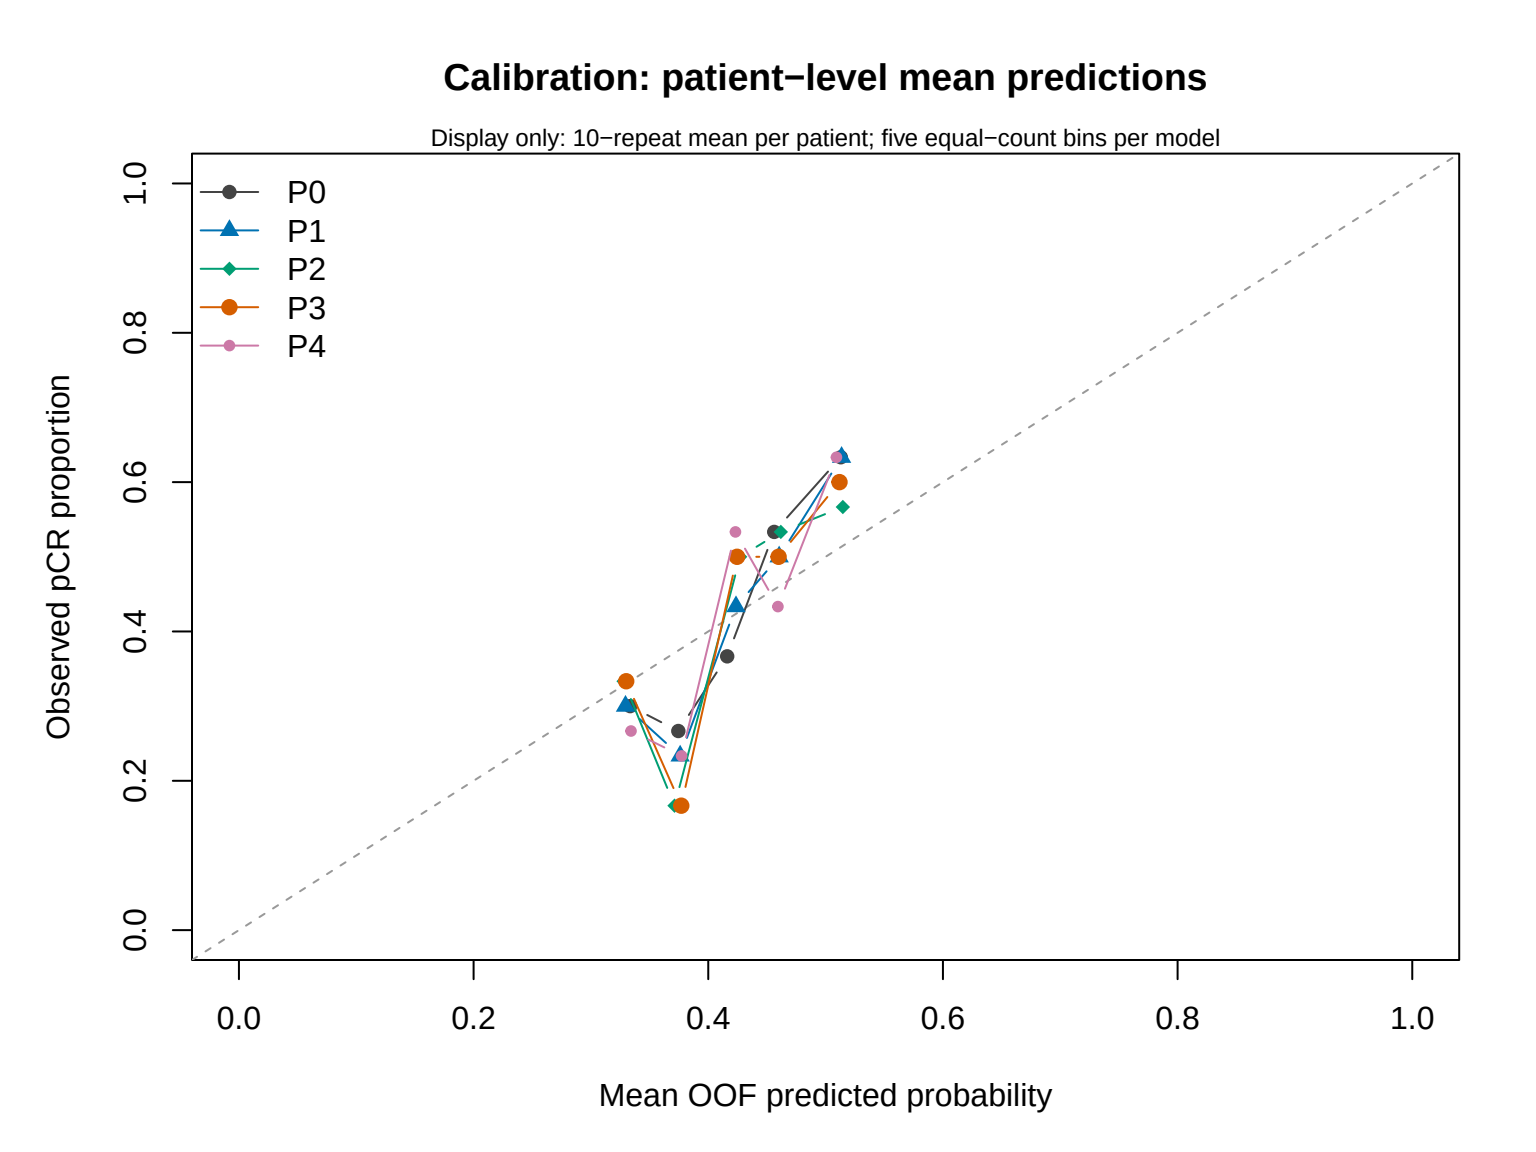
Calibration: patient−level mean predictions
Display only: 10−repeat mean per patient; five equal−count bins per model
P0
P1
P2
P3
P4
Observed pCR proportion
Mean OOF predicted probability
0.0
0.2
0.4
0.6
0.8
1.0