This is a special file, named RPTHEAD.TXT, in the directory of a method
which allows you to customize the report header page.
It can be used to identify the laboratory which uses the method.

This file is printed on the first page with the report styles:

Header+Short, GLP+Short, GLP+Detail, Short+Spec, Detail+Spec, Full

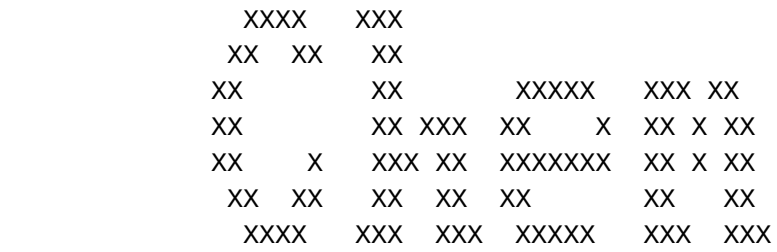

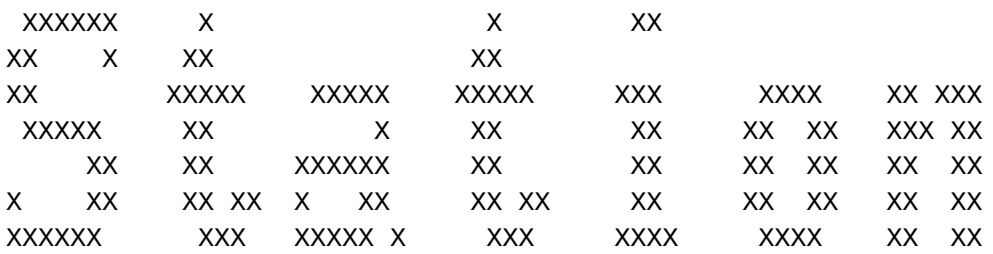

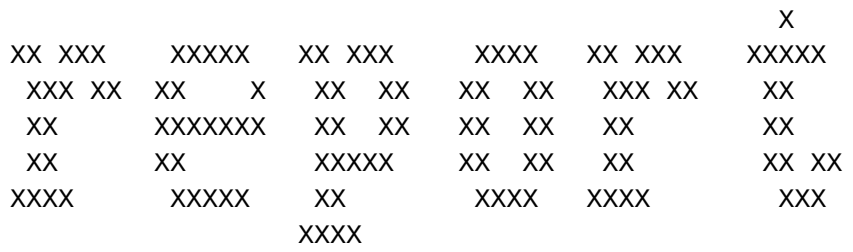

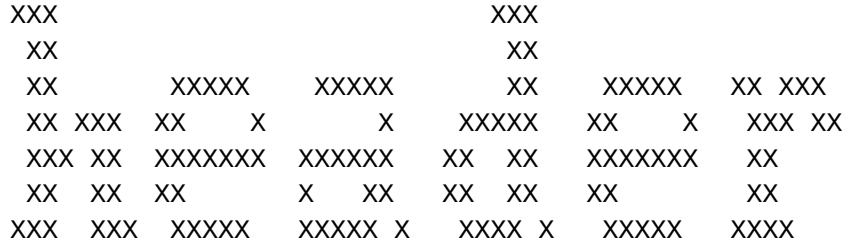

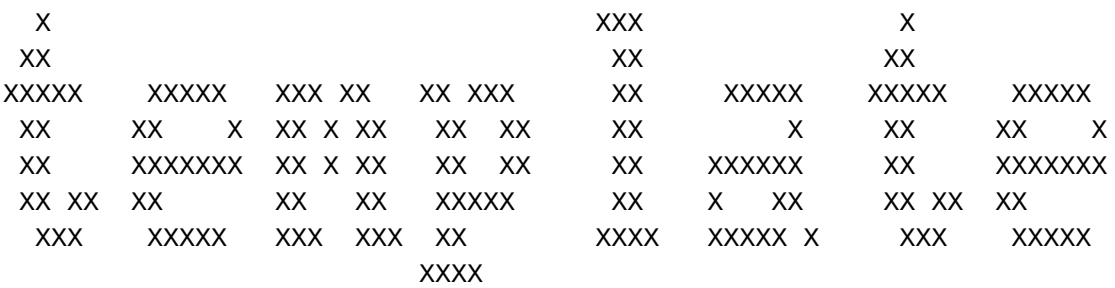

```
==================================================================
Acq. Operator   :                                  Seq. Line :   4
Acq. Instrument : Kortemmelab HPLC                  Location : Vial 1
Injection Date  : 11/17/2020 11:40:43 PM                 Inj :   1
                                                  Inj Volume : 100.0 µl
Sequence File   : C:\Chem32\1\DATA\20201117_GSP1_S75_WITH_STANDARD 2020-11-17 21-00-45\
                  20201117_GSP1_S75_WITH_STANDARD.S
Method          : C:\CHEM32\1\DATA\20201117_GSP1_S75_WITH_STANDARD 2020-11-17 21-00-45\CJM_
                  S75_RUN_ISOCRATIC.M (Sequence Method)
Last changed    : 11/12/2020 5:53:30 PM
Method Info     : S75 analytical

==================================================================
Module                                 Type   Firmware rev.   Serial number
---------------------------------------|------|---------------|---------------
1200 Autosampler SL                    G1329B A.06.54 [003]   DE64155932
1200 Multiple Wavelength Detector      G1365D B.06.72 [0002]  DE64256327
1100/1200 Quaternary Pump              G1311A A.06.32 [011]   DE62971812
1200 Sample Thermostat                 G1330B n/a             DEBAK15882

Software Revision: Rev. B.04.03 [16] Copyright © Agilent Technologies
==================================================================
                              Column(s)
==================================================================

Column Description :  Sephadex 75, 10/300
Serial#            :  10108795
Product#           :  17-5174-01        Batch# :
Diameter           :  4.6 mm           Length :  150.0 mm
Particle size      :  5.0 µm      Void volume :   60.0 %
# Injections       :   74
Maximum Pressure   :   18.0 bar      Maximum pH :      9.0
     Minimum pH :      2.0
Maximum Temperature:   60.0 °C
Comment            :
==================================================================

Instrument Conditions   :    At Start           At Stop
Pressure                :       0.0              15.7   bar
Flow                    :       0.000             0.800 ml/min

Detector Lamp Burn Times: Current On-Time  Accumulated On-Time

Solvent Description     :
PMP1 , Solvent A        : ddH20
PMP1 , Solvent B        : EtOH
PMP1 , Solvent C        : Tris NaCl
PMP1 , Solvent D        :
```

Data File C:\CHEM32\...01117_GSP1_S75_WITH_STANDARD 2020-11-17 21-00-45\20201117_BLANK_2.D
Sample Name: Blank_2

==========

Run Logbook

==========

18 Nov 20 00:14 AM
Logbook File:C:\Chem32\...TANDARD 2020-11-17 21-00-45\20201117_BLANK_2.D\RUN.LOG

Module	# Event Message	Time	Date
Method	Method started: line# 4 vial# 1 inj# 1	23:40:32	11/17/20
Method	Instrument running sample Vial 1	23:40:32	11/17/20
ALS	Air temperature (tray) = 4.0 °C	23:43:56	11/17/20
PUMP	Pressure = 0.0 bar	23:43:56	11/17/20
PUMP	Flow = 0.000 ml/min	23:43:56	11/17/20
PUMP	Pressure = 15.7 bar	00:13:56	11/18/20
Method	Instrument run completed	00:13:59	11/18/20
Method	Saving Method CJM_S75_RUN_ISOCRATIC.M	00:14:00	11/18/20
Method	Saving Method RUN.M	00:14:02	11/18/20
CP Macro	Analyzing rawdata 20201117_BLANK_2.D	00:14:02	11/18/20
CP Macro	Can't load MWD1 D, Sig=230,8 Ref=360,100	00:14:02	11/18/20
CP Macro	Signal used in Calib. Table (Signal Details)>	00:14:02	11/18/20
	.		

==========

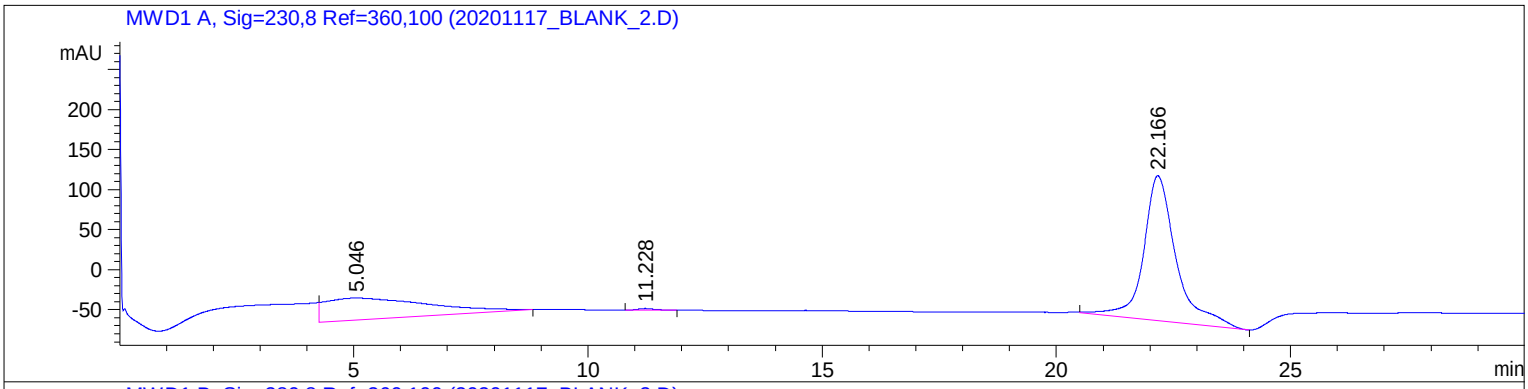

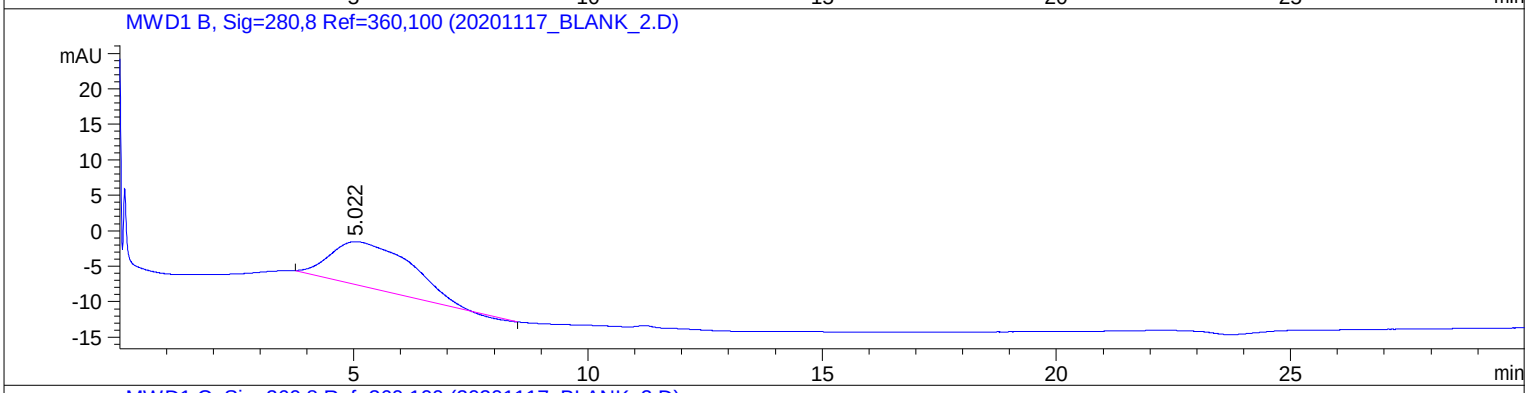

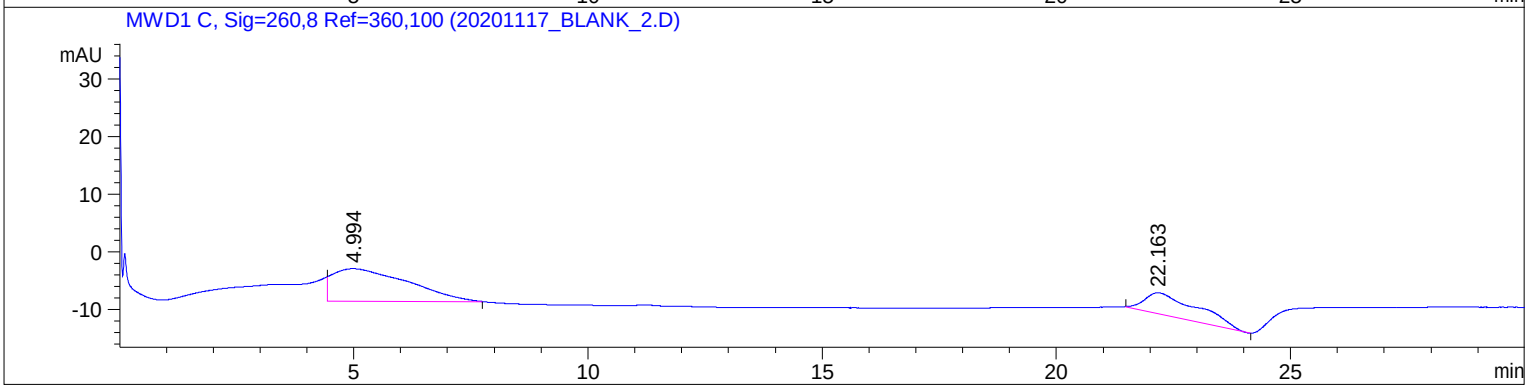

Data File C:\CHEM32\...01117_GSP1_S75_WITH_STANDARD 2020-11-17 21-00-45\20201117_BLANK_2.D
Sample Name: Blank_2

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: MWD1 A, Sig=230,8 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.046	BB	1.7583	4046.71216	27.19163	31.5217
2	11.228	BB	0.3307	43.54779	1.90517	0.3392
3	22.166	BV	0.7088	8747.59375	181.33812	68.1391
Totals :				1.28379e4	210.43492	

Signal 2: MWD1 B, Sig=280,8 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.022	BB	1.5075	771.84570	6.03736	100.0000
Totals :				771.84570	6.03736	

Signal 3: MWD1 C, Sig=260,8 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.994	BB	1.3343	633.97394	5.63639	67.3341
2	22.163	BV	1.0767	307.56110	3.62931	32.6659
Totals :				941.53503	9.26570	

==========

*** End of Report ***