

Liver FibroScan (Elastography)

肝纤维瞬时弹性+脂肪变

Patient: Lei Zhu (Clark) · Male · DOB 1992-06-23 | Exam date: 2026-04-01 | Southwest Hospital Health Management Center, Chongqing | Check-up ID: 8002262907

Liver Transient Elastography (FibroScan) / 肝纤维瞬时弹性+脂肪变测定

Test	项目	Result	Reference	Unit	Flag
CAP (steatosis)	脂肪变 CAP	311	>=292 severe (>=67% fat)	dB/m	High ↑
E (stiffness)	硬度 E	5.2	<7.3 normal (F0-F1)	kPa	
Valid / total measurements	有效/总测量	12 / 12	-		
CAP IQR	CAP四分位距	34	-	dB/m	
E IQR / median	E离散度	21	<30	%	

Interpretation / 解读

CAP 311 dB/m — severe hepatic steatosis (fatty liver, ≥67% of hepatocytes). **E 5.2 kPa — normal liver stiffness** (no significant fibrosis, stage F0–F1). Probe M, device 502TOUCH.

CAP 311 dB/m 提示重度脂肪肝 (≥67%)。E 5.2 kPa 提示肝脏硬度正常 (无明显纤维化, F0–F1)。

The original examination image/waveform is appended on the following page(s). 原始检查图像/波形见后页。

English translation prepared for clinical reference (bilingual). Source: Southwest Hospital / Army Medical University First Affiliated Hospital, Chongqing, China — annual health check-up 2026-04-01. Values transcribed from the original Chinese report; if any discrepancy arises, the original report prevails.



陆军军医大学第一附属医院

肝脏瞬时弹性硬度值及脂肪变检测报告单

检查时间：2026年04月01日 09时03分

姓名：朱雷

性别：男

年龄：33岁

申请医生：

门诊号：8002262907

申请科室：体检中心

CAP[dB/m]

E[kPa]

IQR

34

311

中值

5.2

IQR

1.1


IQRV

21%

检查类型：M

有效测量：12

总计测量：12

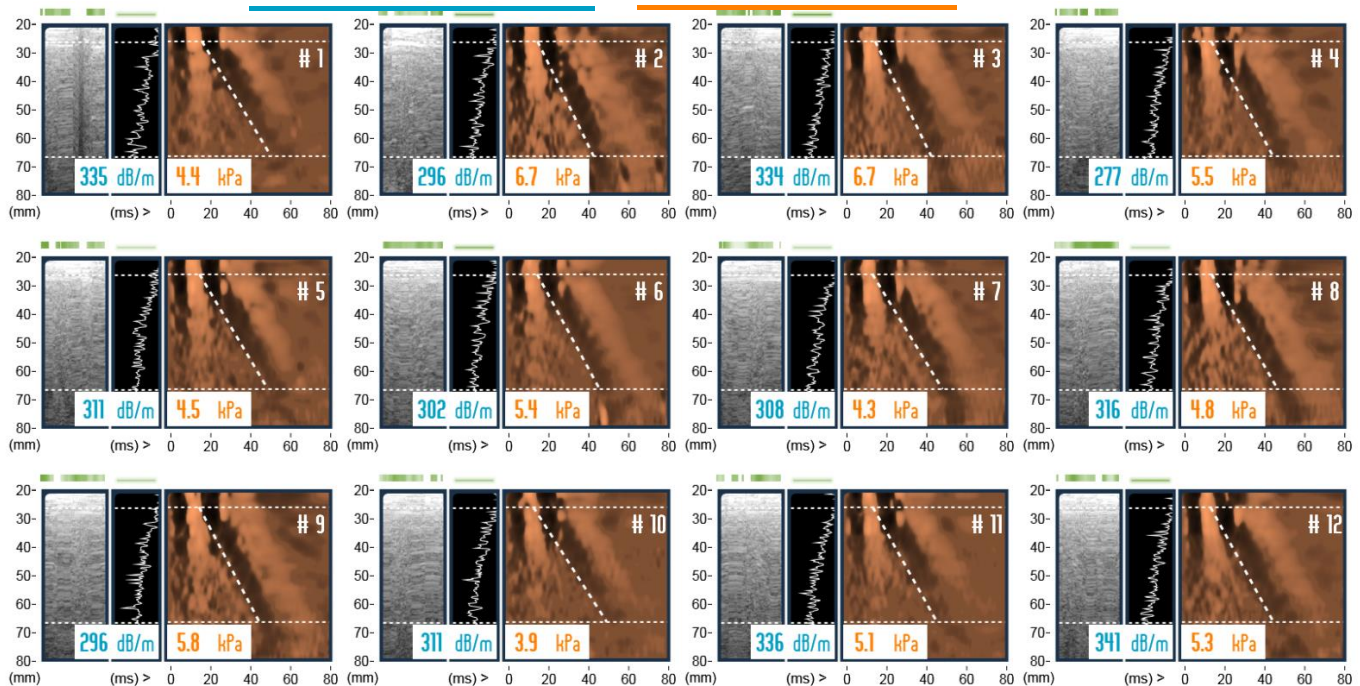

CAP值与组织病理学分期对照参考标准

脂肪变≤10%

238

脂肪变≥11%

259

脂肪变≥34%

292

脂肪变≥67%

CAP[dB/m]

肝脏硬度值与组织病理学分期对照参考标准

F0F1

7.3

F2

9.7

F2F3

12.4

F3F4

17.5

F4

E[kPa]

*此报告仅供临床参考，不作为最终诊断结果

操作员：

陈有为

FibroScan® 检查设备型号：502TOUCH 检查设备序列号：F62486

是一款用于辅助管理肝病患者的医疗设备。本设备必须由经过本公司认证的操作员进行操作。通过本设备获取的测量结果必须由专业的肝病医师结合患者的病情、有效测量数和测量结果的离散度来解读。VCTE探头必须根据制造商的建议定期校准。

echosens