

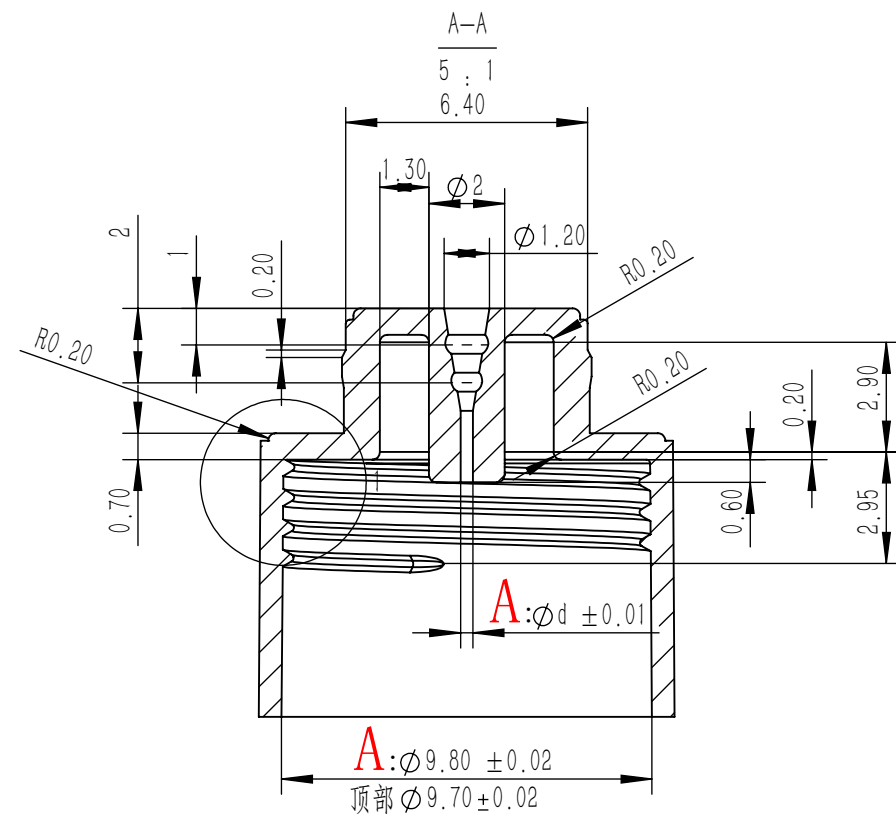
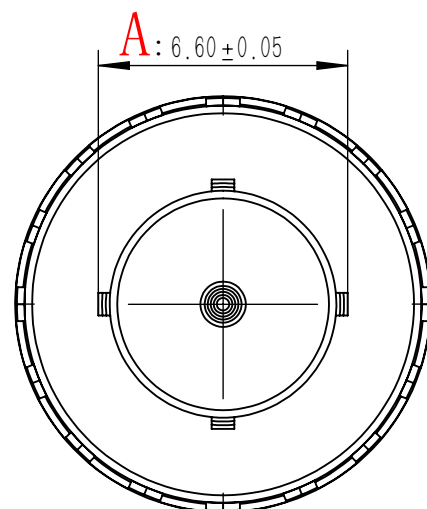
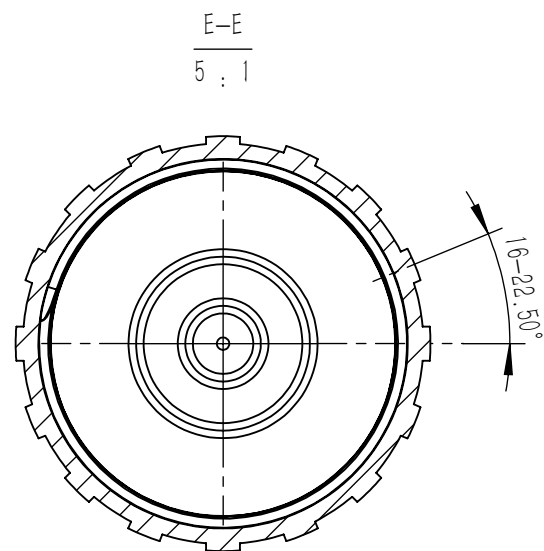


03-03-0101

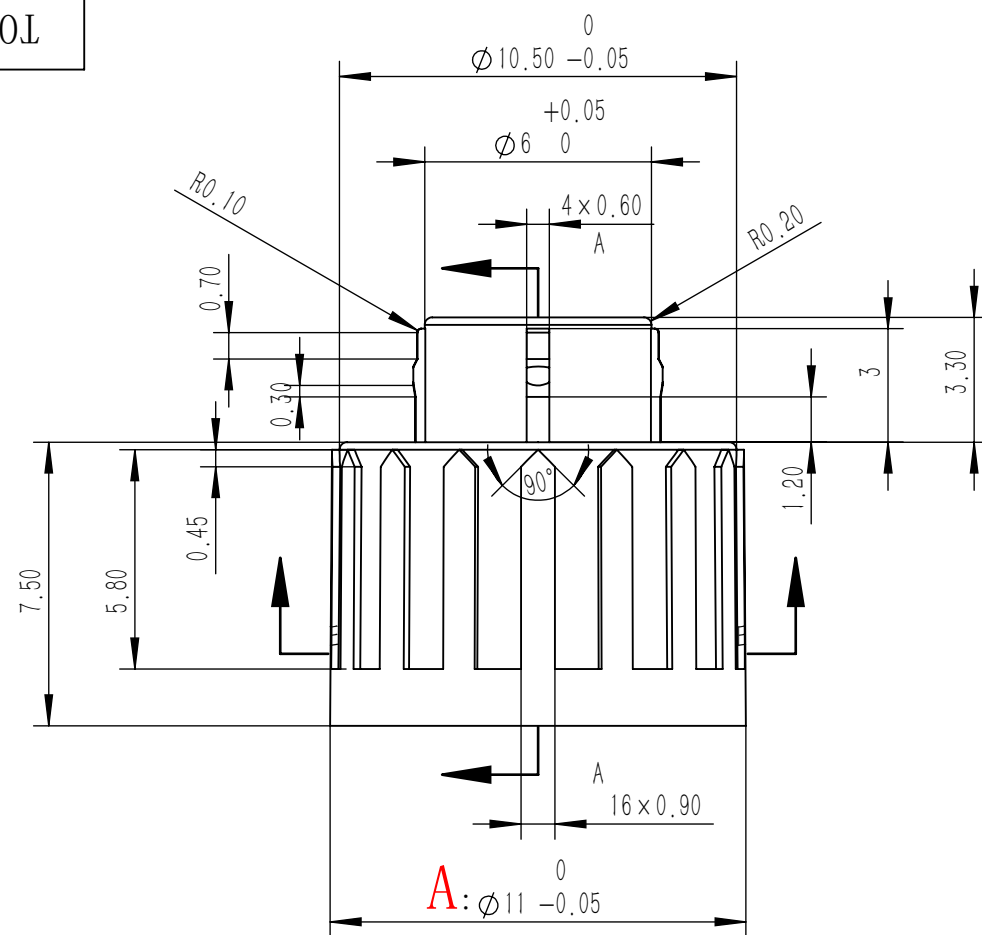

Size	Needle OD	d
27G / 0.40	0.41 ± 0.01	0.43

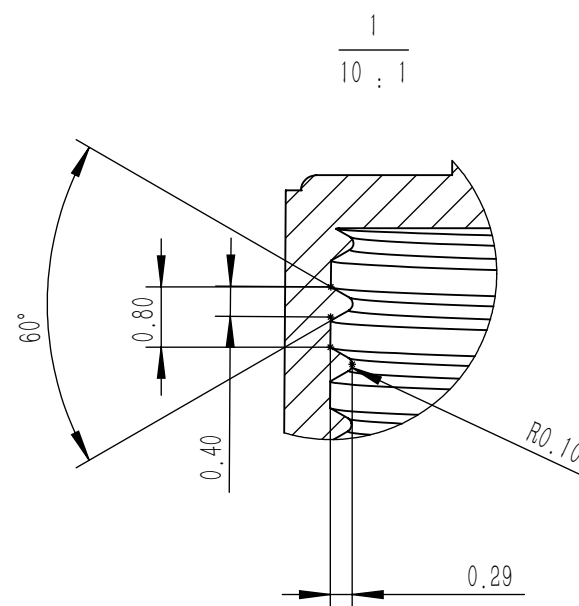

Technical department:

1. The component should be no burr, edge, missing or deformation etc;
2. The component should match with small protective cover well without naturally fallen;
3. The screw of this part should match with insulin syringe well without fallen
4. The screw is ballet screw, the thread pitch is 0.8;
5. A is key dimension.

				名称 Title	图号 Drawing No.							
					T010-03-03							
					Needle hub for 27G pen needle	未注公差要求 Tolerances Unless Otherwise Specified:	≤3	>3~≤6	>6~≤15	>15~≤30	>30	版本Ver
更改单号 Change order No.	更改内容 Change Contents		更改人 Changed by				实施日期 Effective Date	±0.05	±0.1	±0.15	±0.2	±0.3
制图 Prepared by		批准 Approved by		材料 Material								
校对 Checked by												
审核 Reviewed by		日期 Date		聚丙烯PP								