


Figure 3. Heatmap of ENDS device use in the CRoFT Study



Follow-up Period

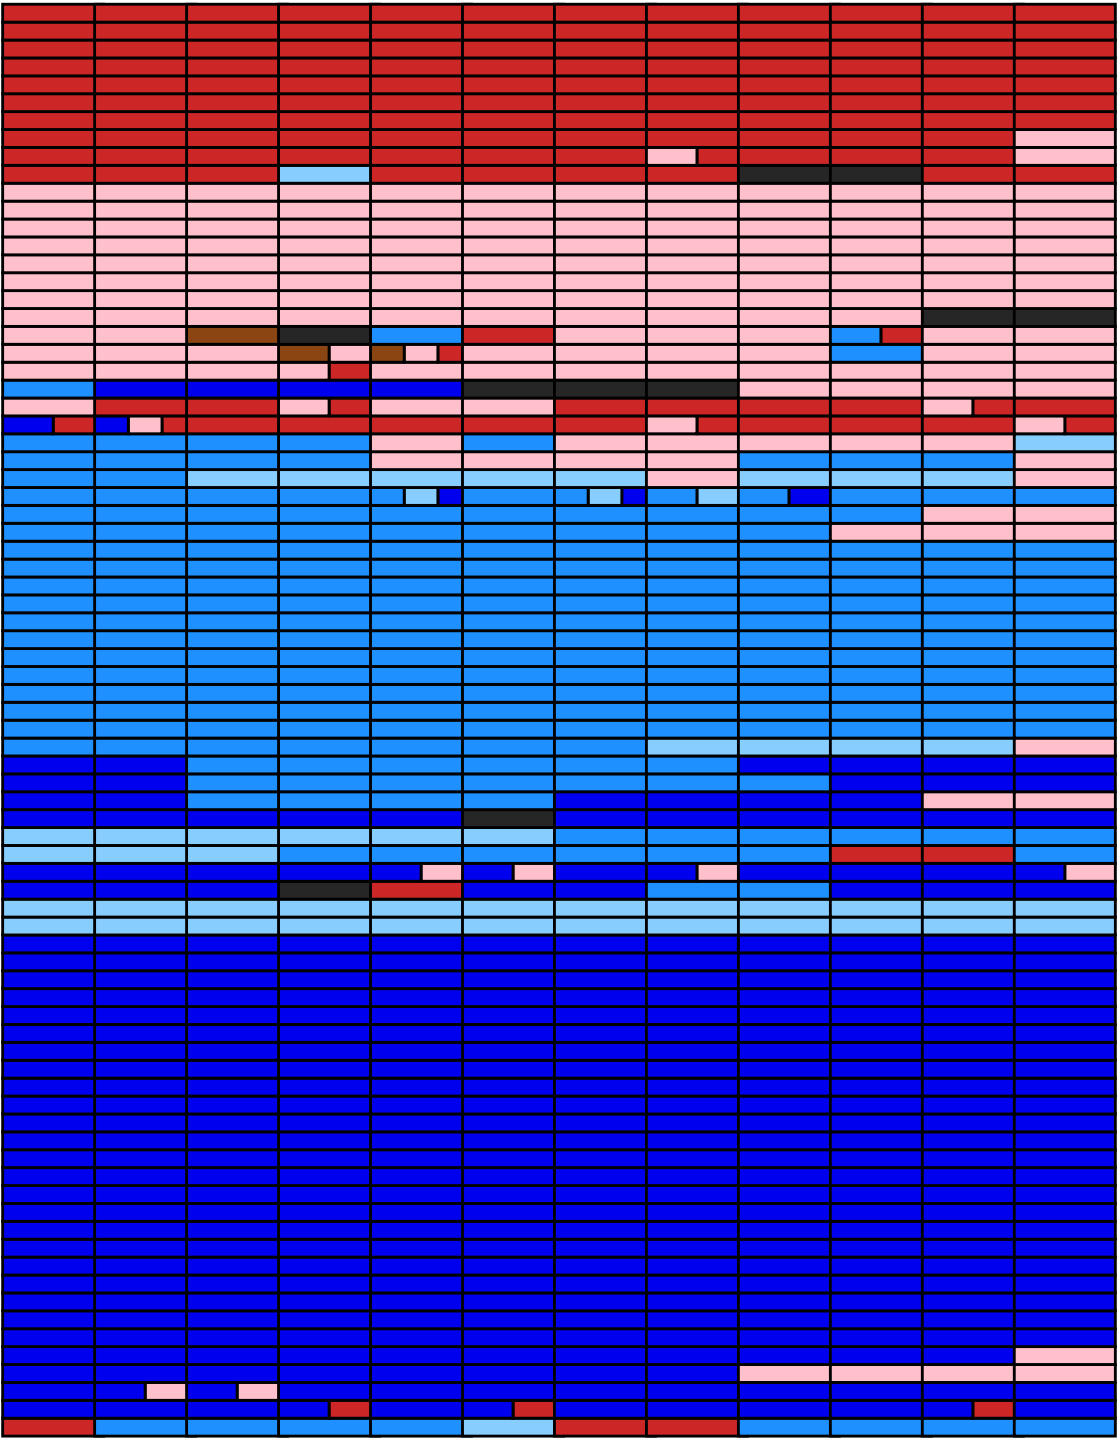