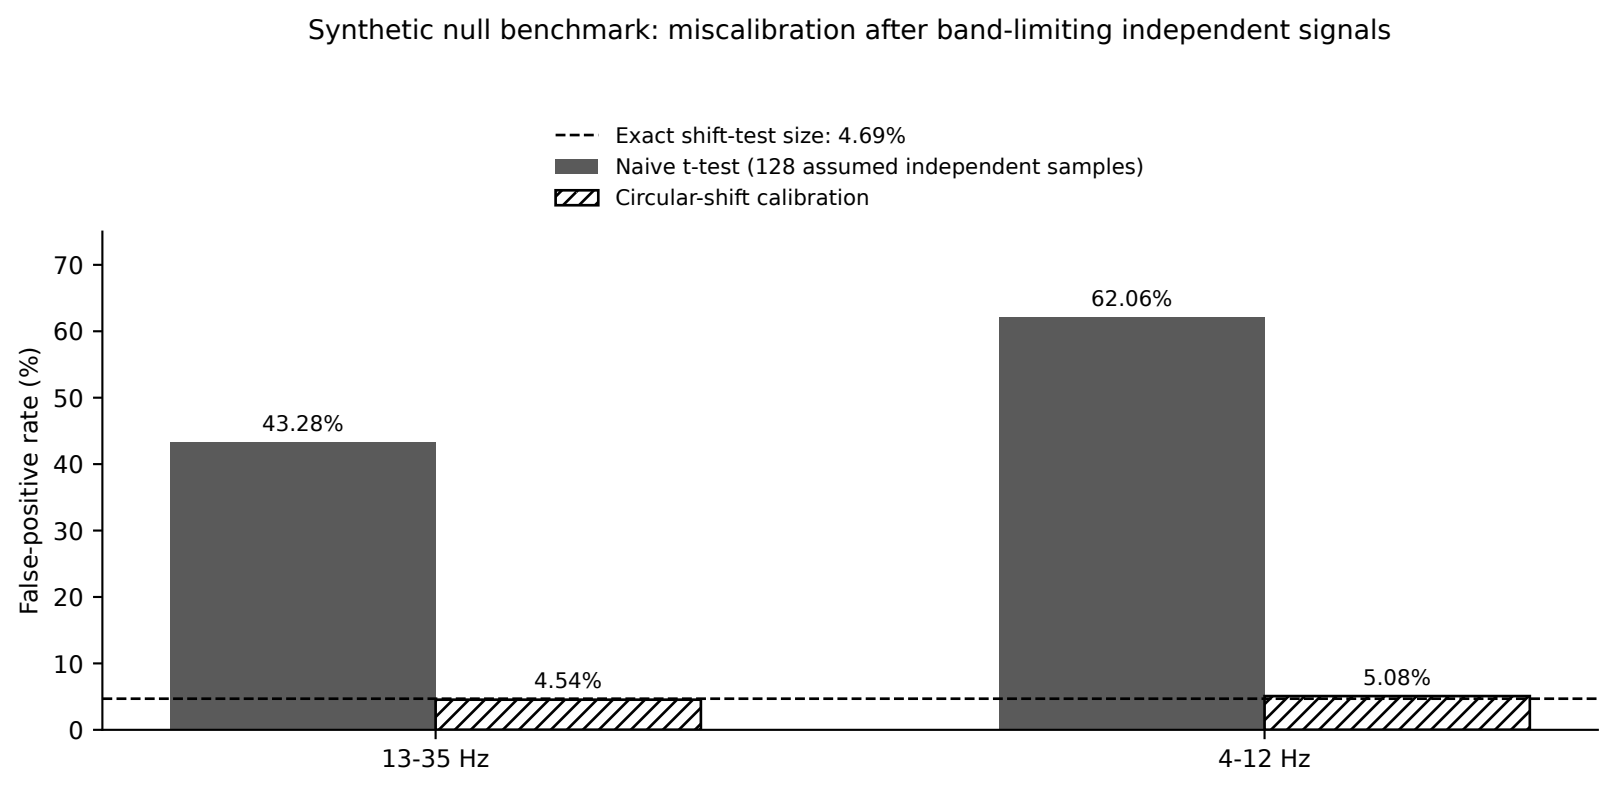
Synthetic null benchmark: miscalibration after band-limiting independent signals
Exact shift-test size: 4.69%
Naive t-test (128 assumed independent samples)
Circular-shift calibration
False-positive rate (%)
0
10
20
30
40
50
60
70
43.28%
4.54%
62.06%
5.08%
13-35 Hz
4-12 Hz