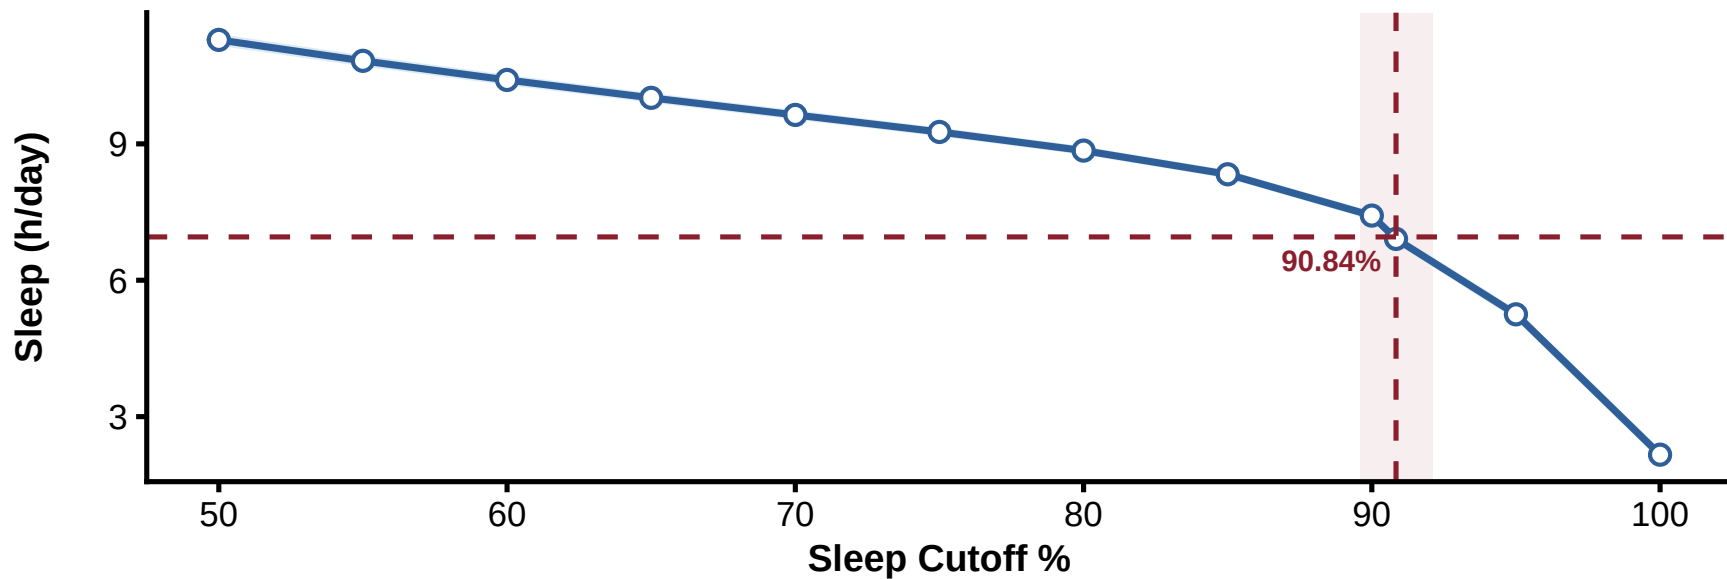


A**Sleep calibration****B****Sedentary-time sensitivity**