


A Sleep-duration calibration



B Sedentary-time sensitivity

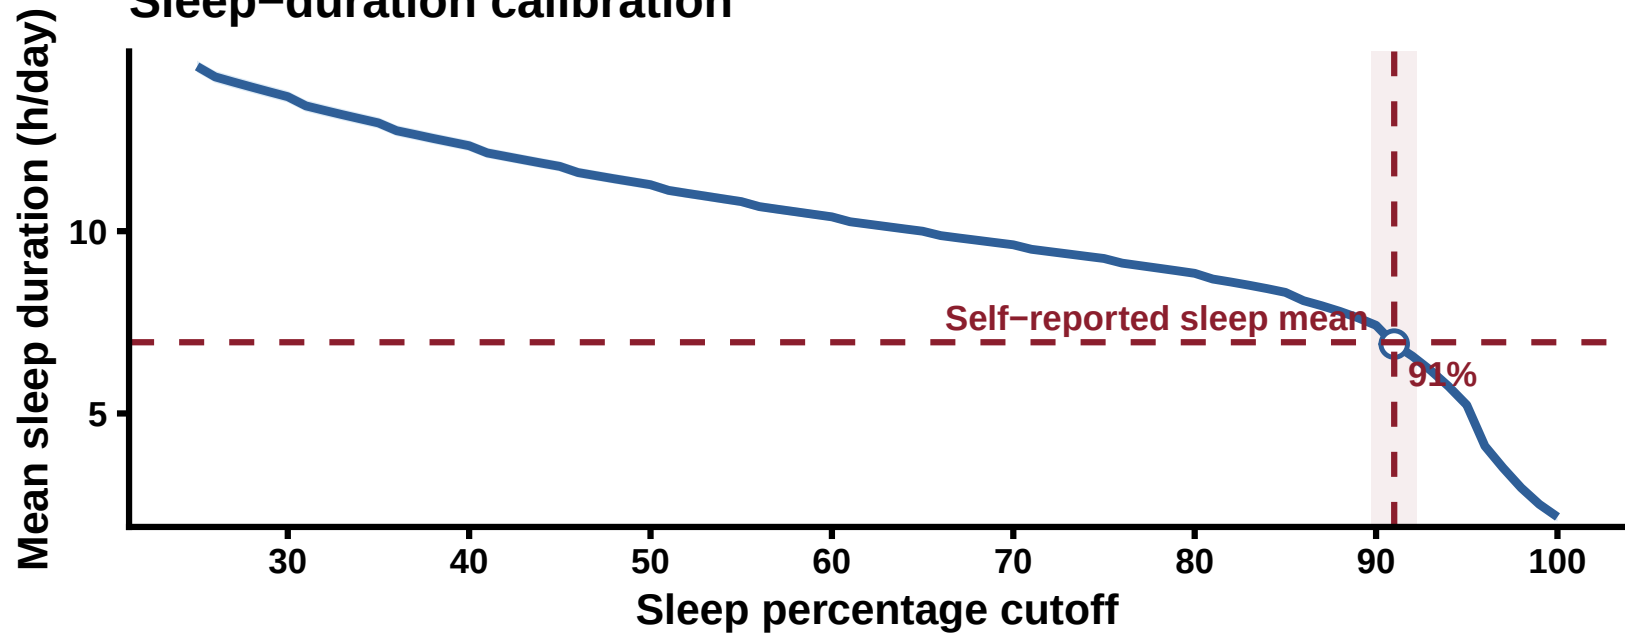