


Figure 15. Calibration diagnostics — raw probabilities are NOT clinically calibrated

(A) Reliability diagram (10 deciles) · HL p=1.8e-04



(B) Decile sample sizes

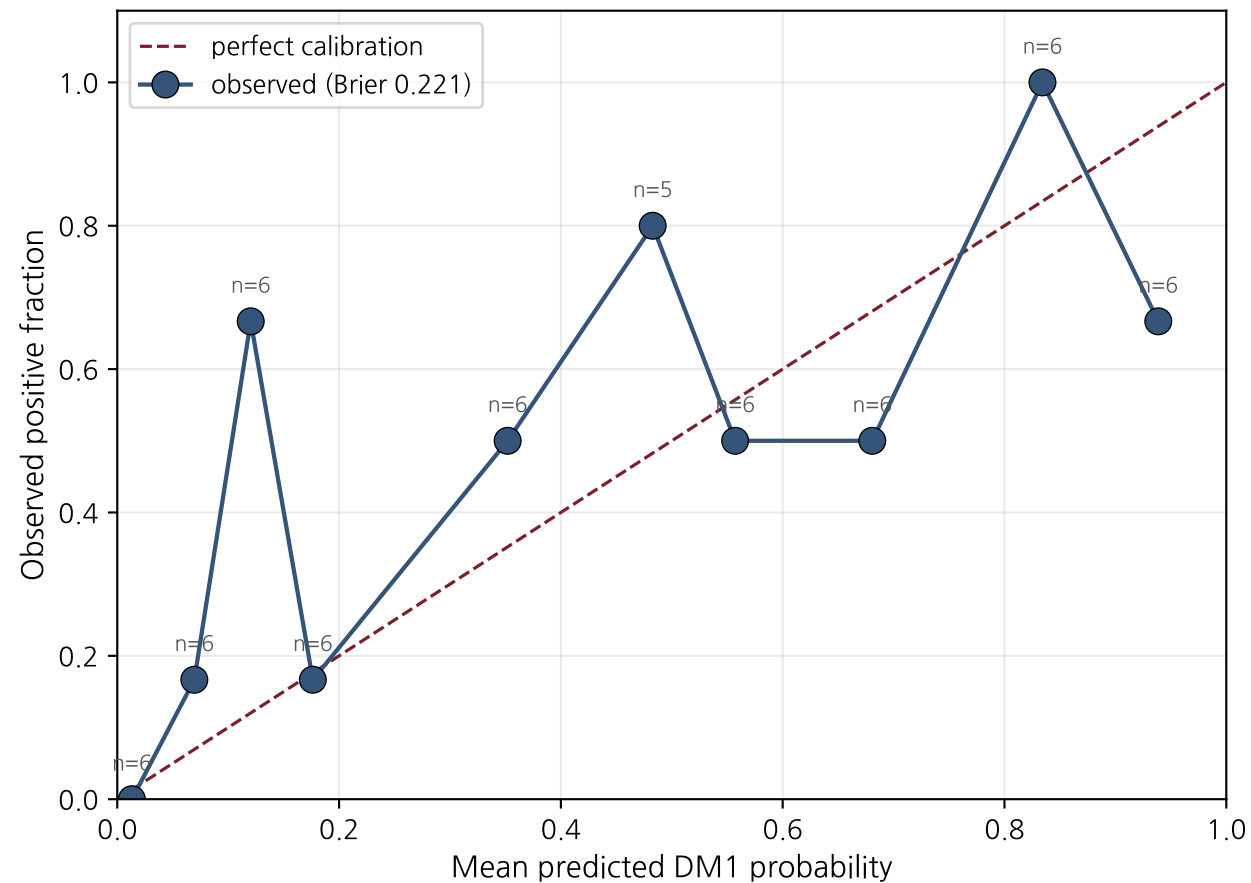