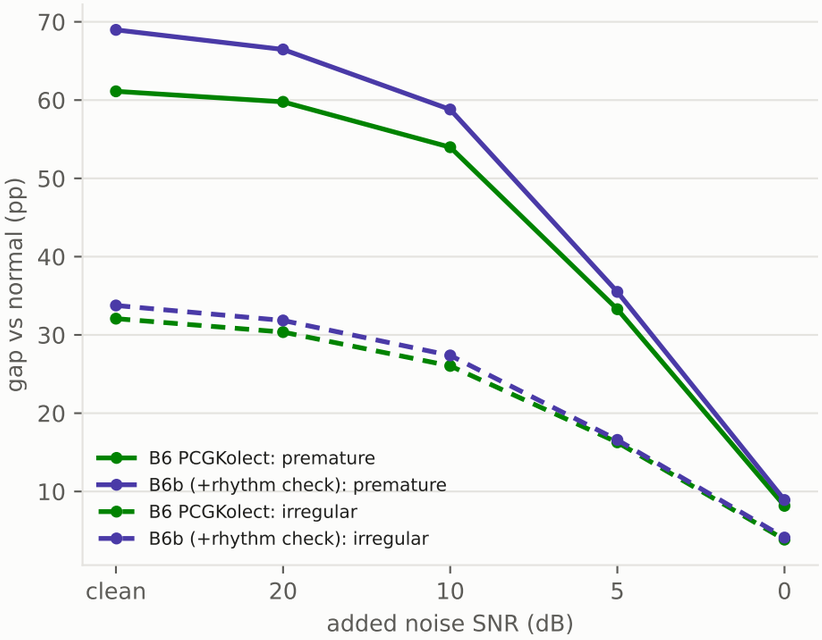

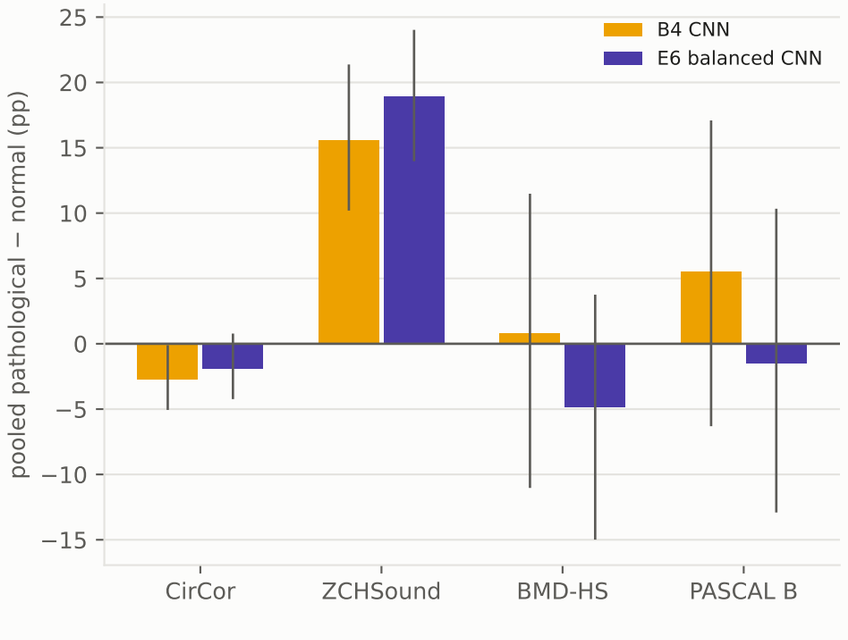

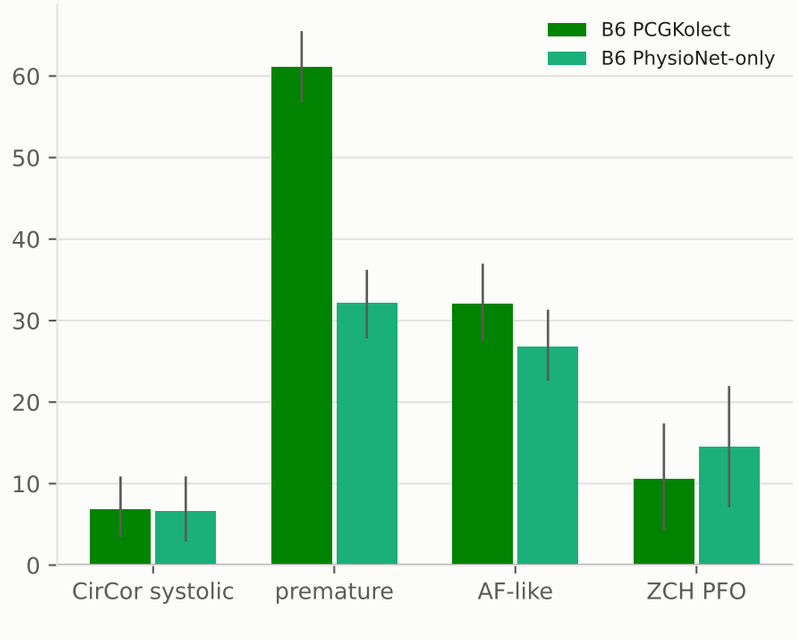

B6 PhysioNet-only matches 77 % of CirCor reference beats vs 99 % for the released checkpoint. 95 % patient-bootstrap CIs.