E1 Raw rejection gap as recorded (all evaluation beats, matched threshold, mean of 3 seeds)

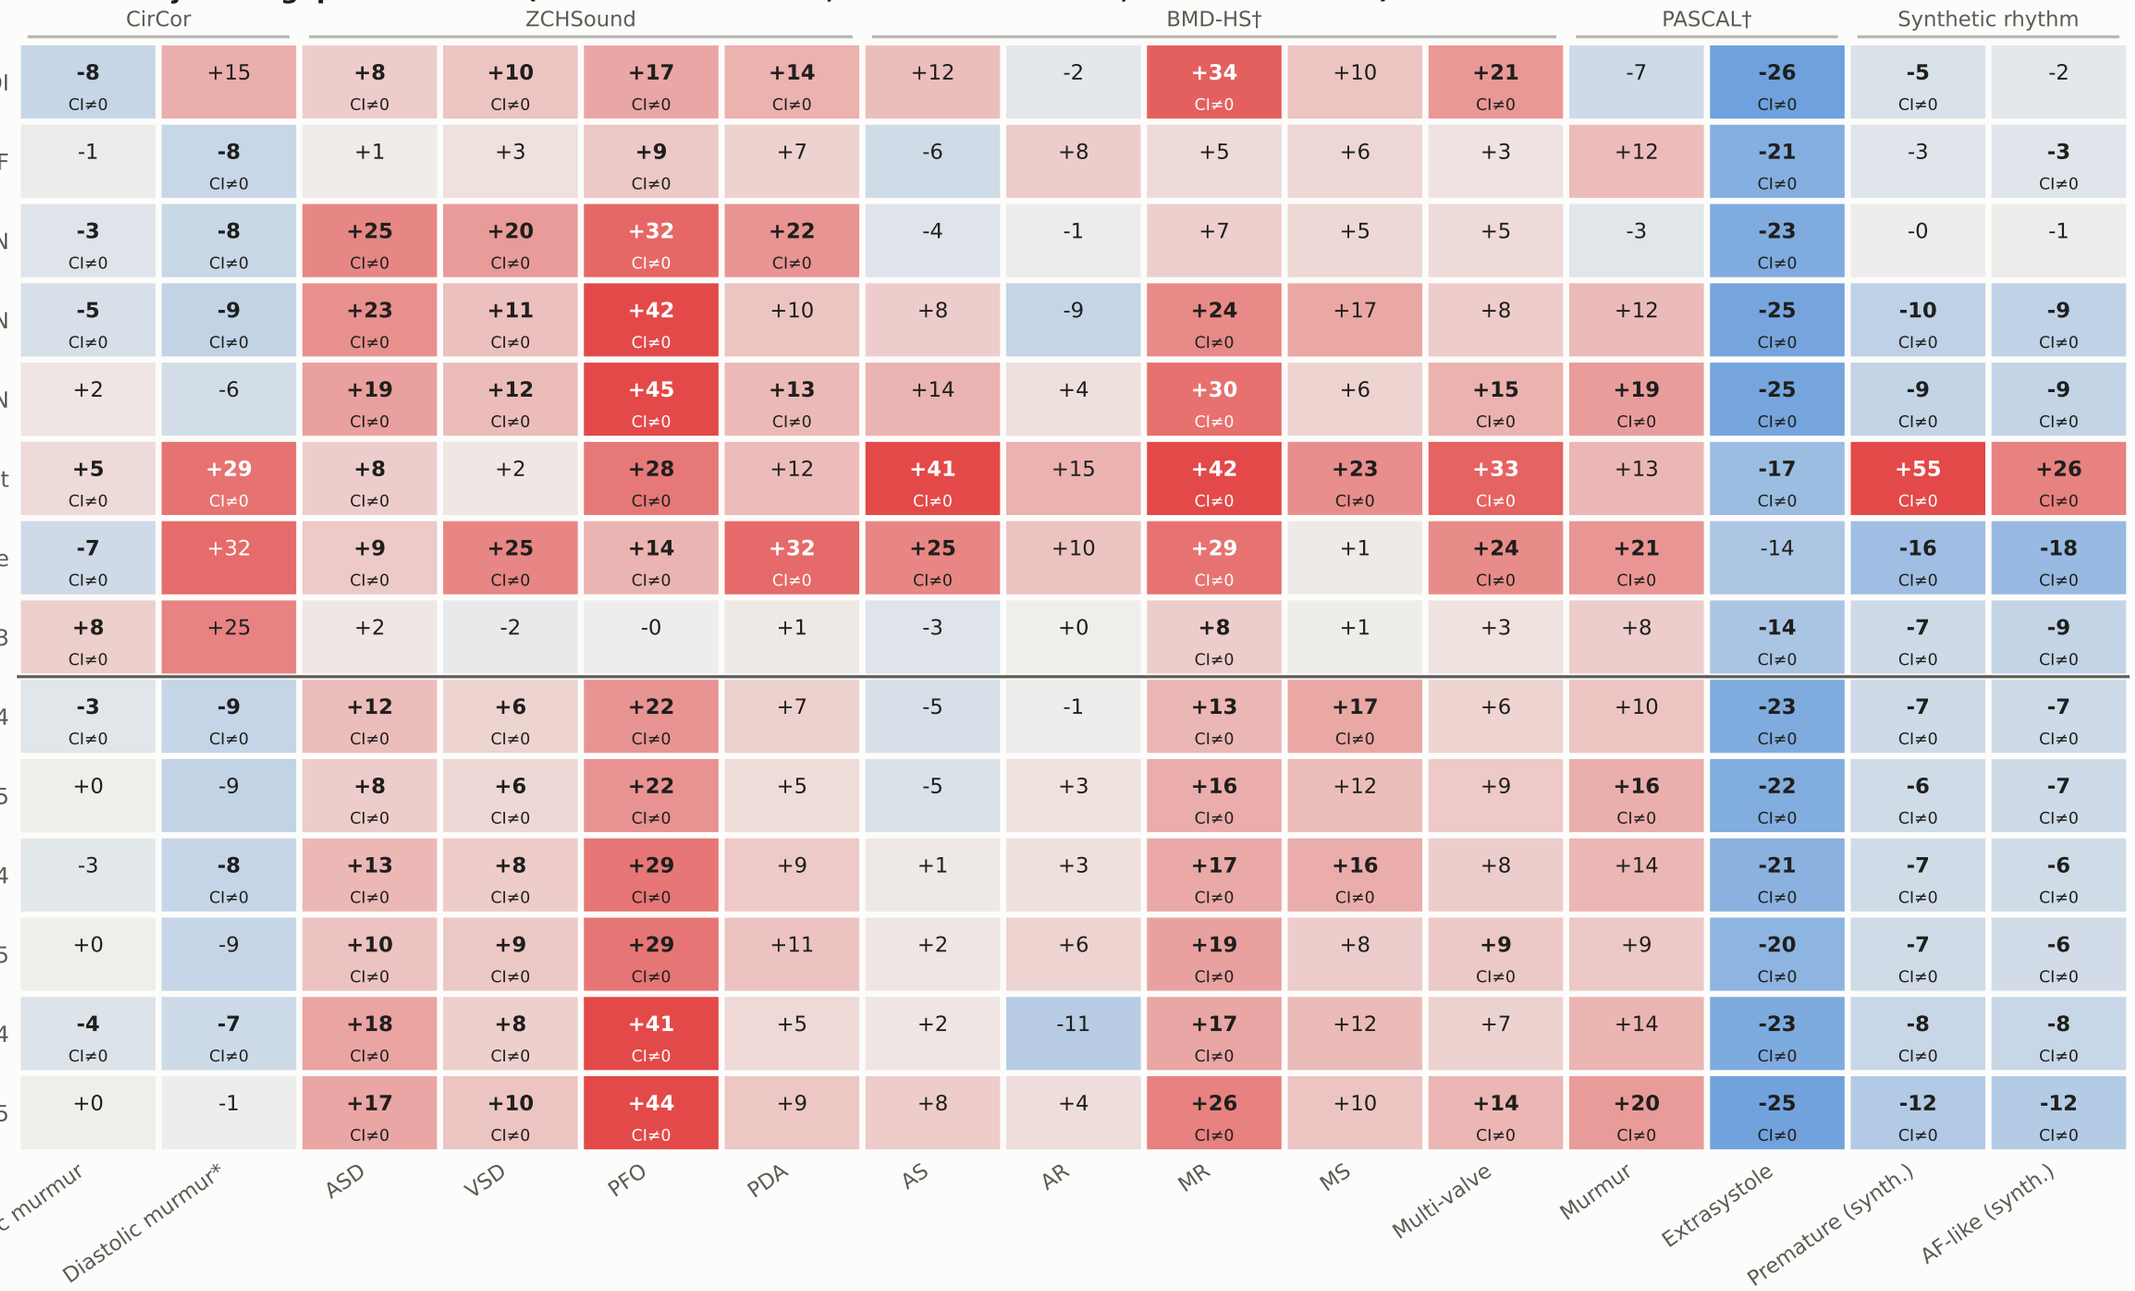

Red = pathology rejected more often than normal beats. Bold/"CI≠0" = 95 % patient-bootstrap CI excludes 0 in ≥ 2 of 3 seeds. * 5 patients. † small calibration sets. E1 mixes recording quality and filter behaviour; E2 isolates the filter. Rows below the line: hybrids.