FIG. 1

Multi-Node Intimate Physiology Monitoring System

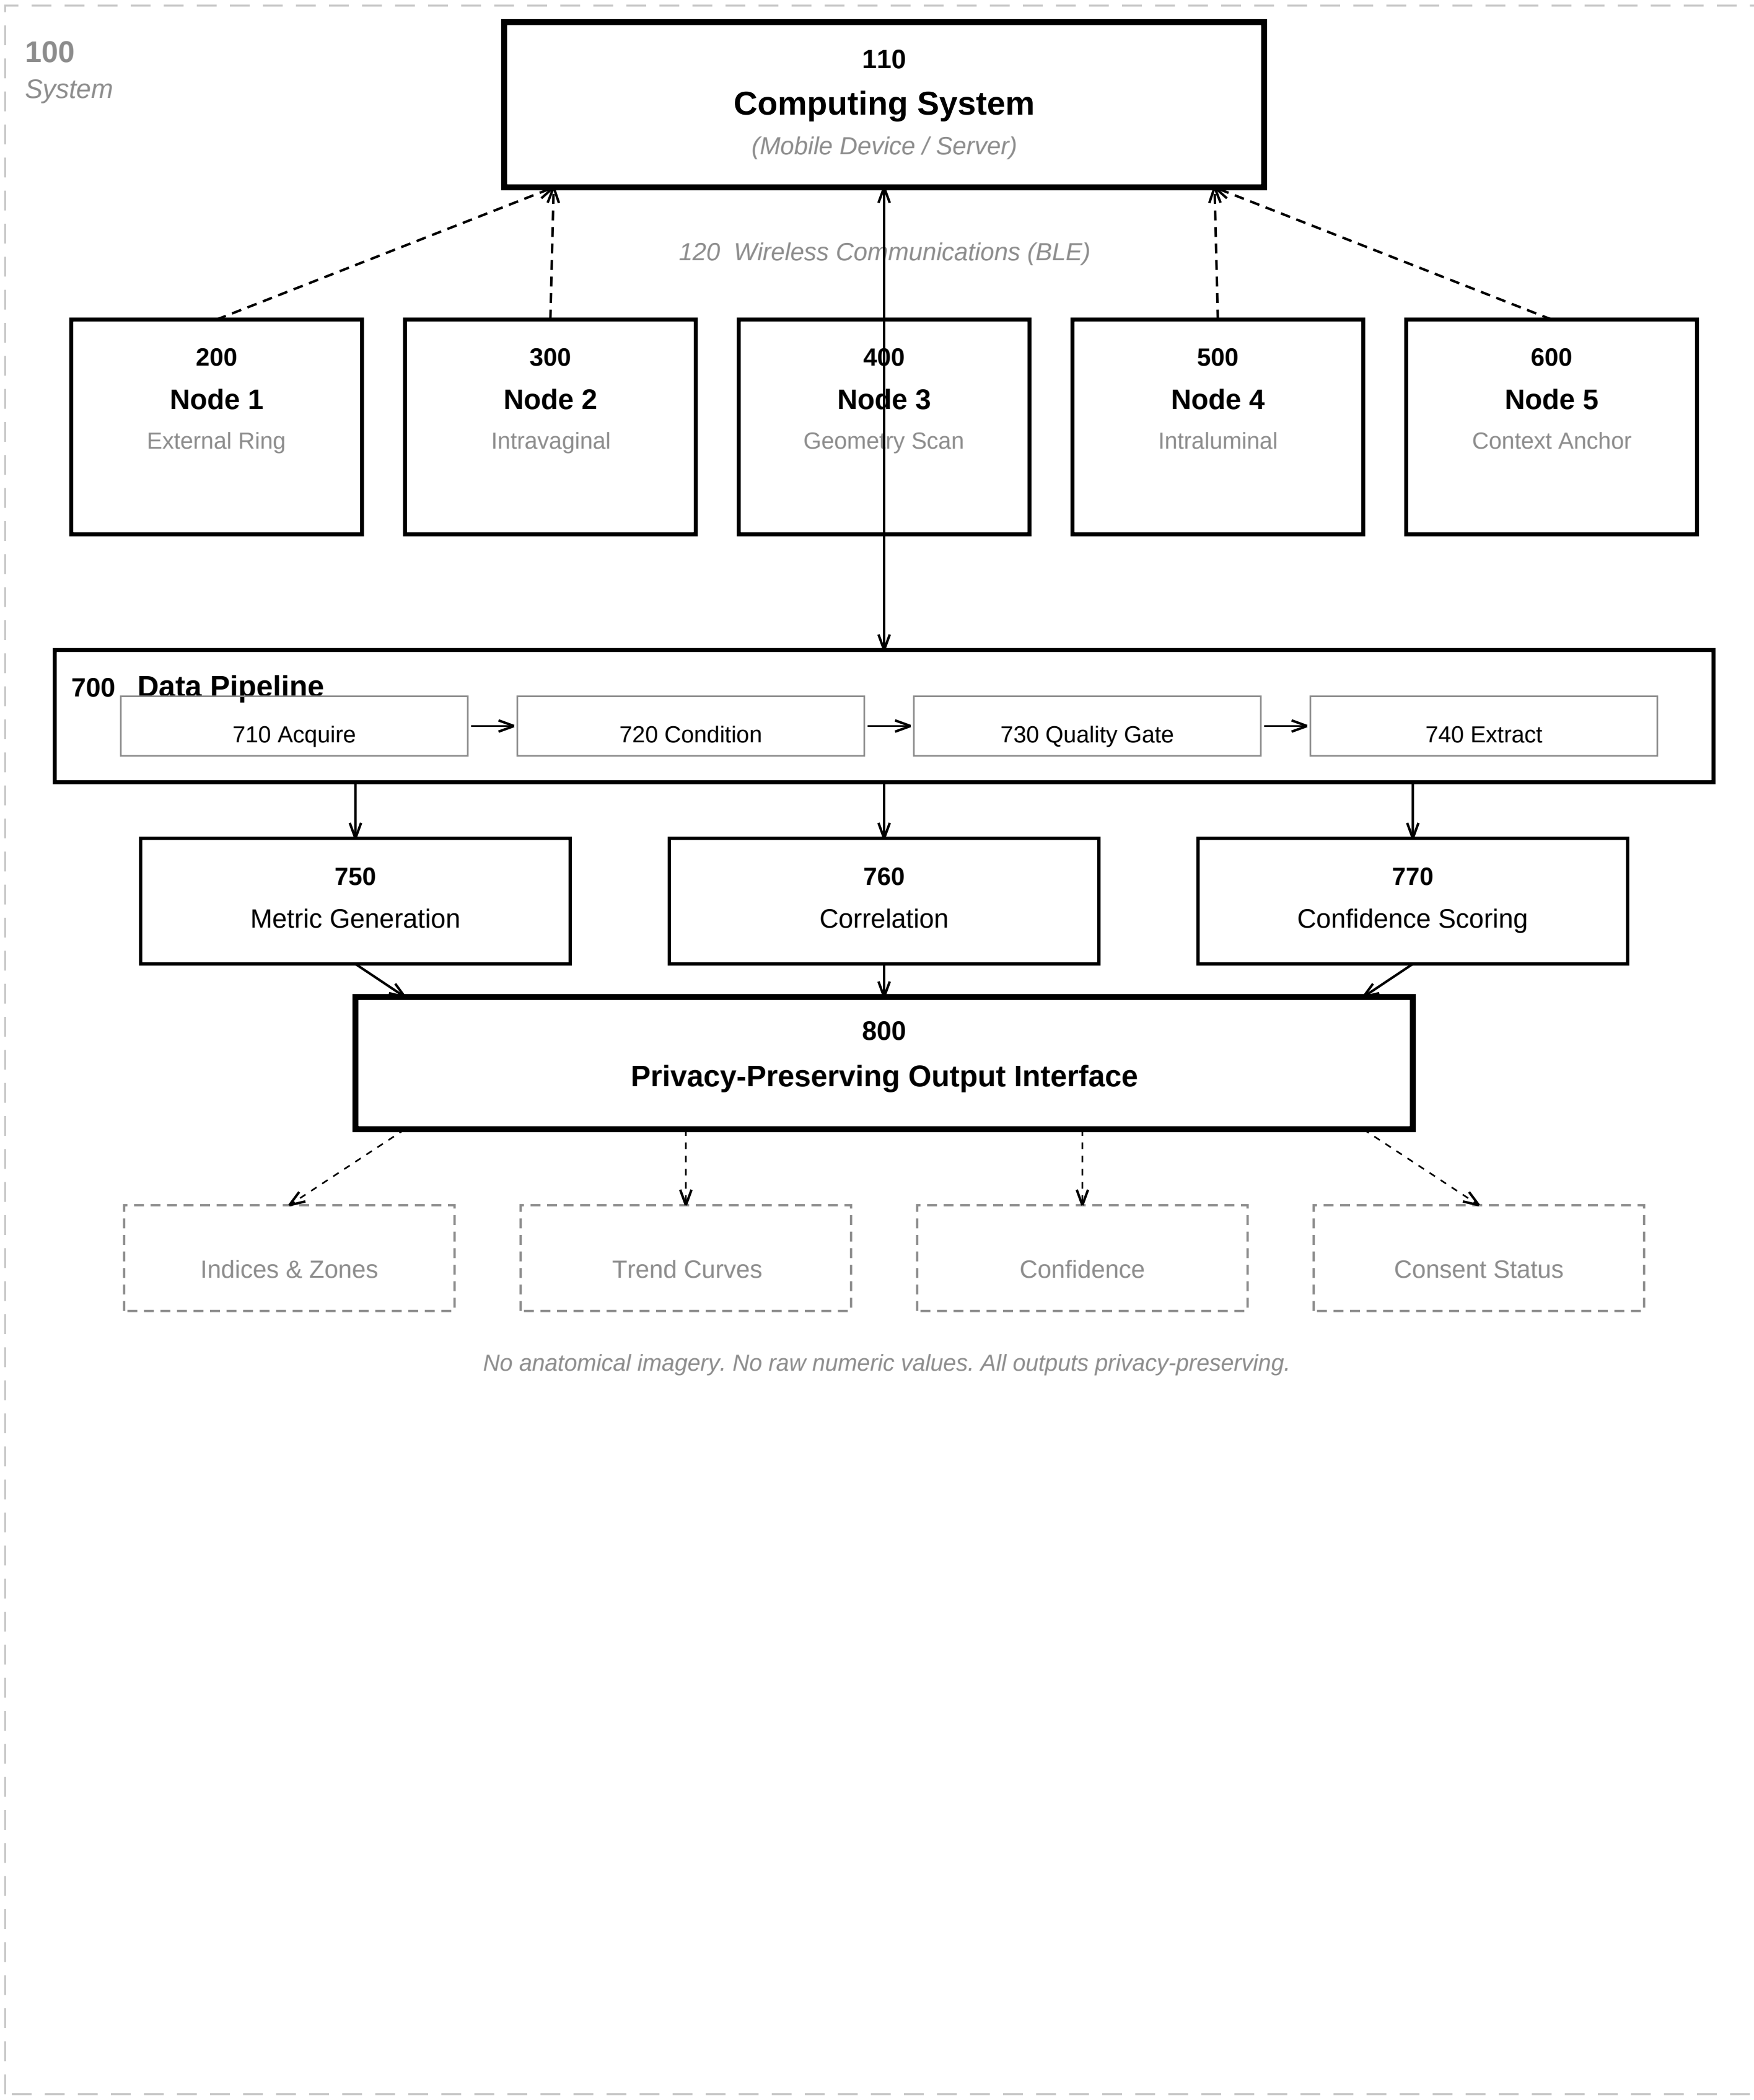

FIG. 2

Node 1 -- External Longitudinal Wearable (Ring Form Factor)

Form Factor A: C-Shape (Open Ring) **Form Factor B: Enclosed Ring**

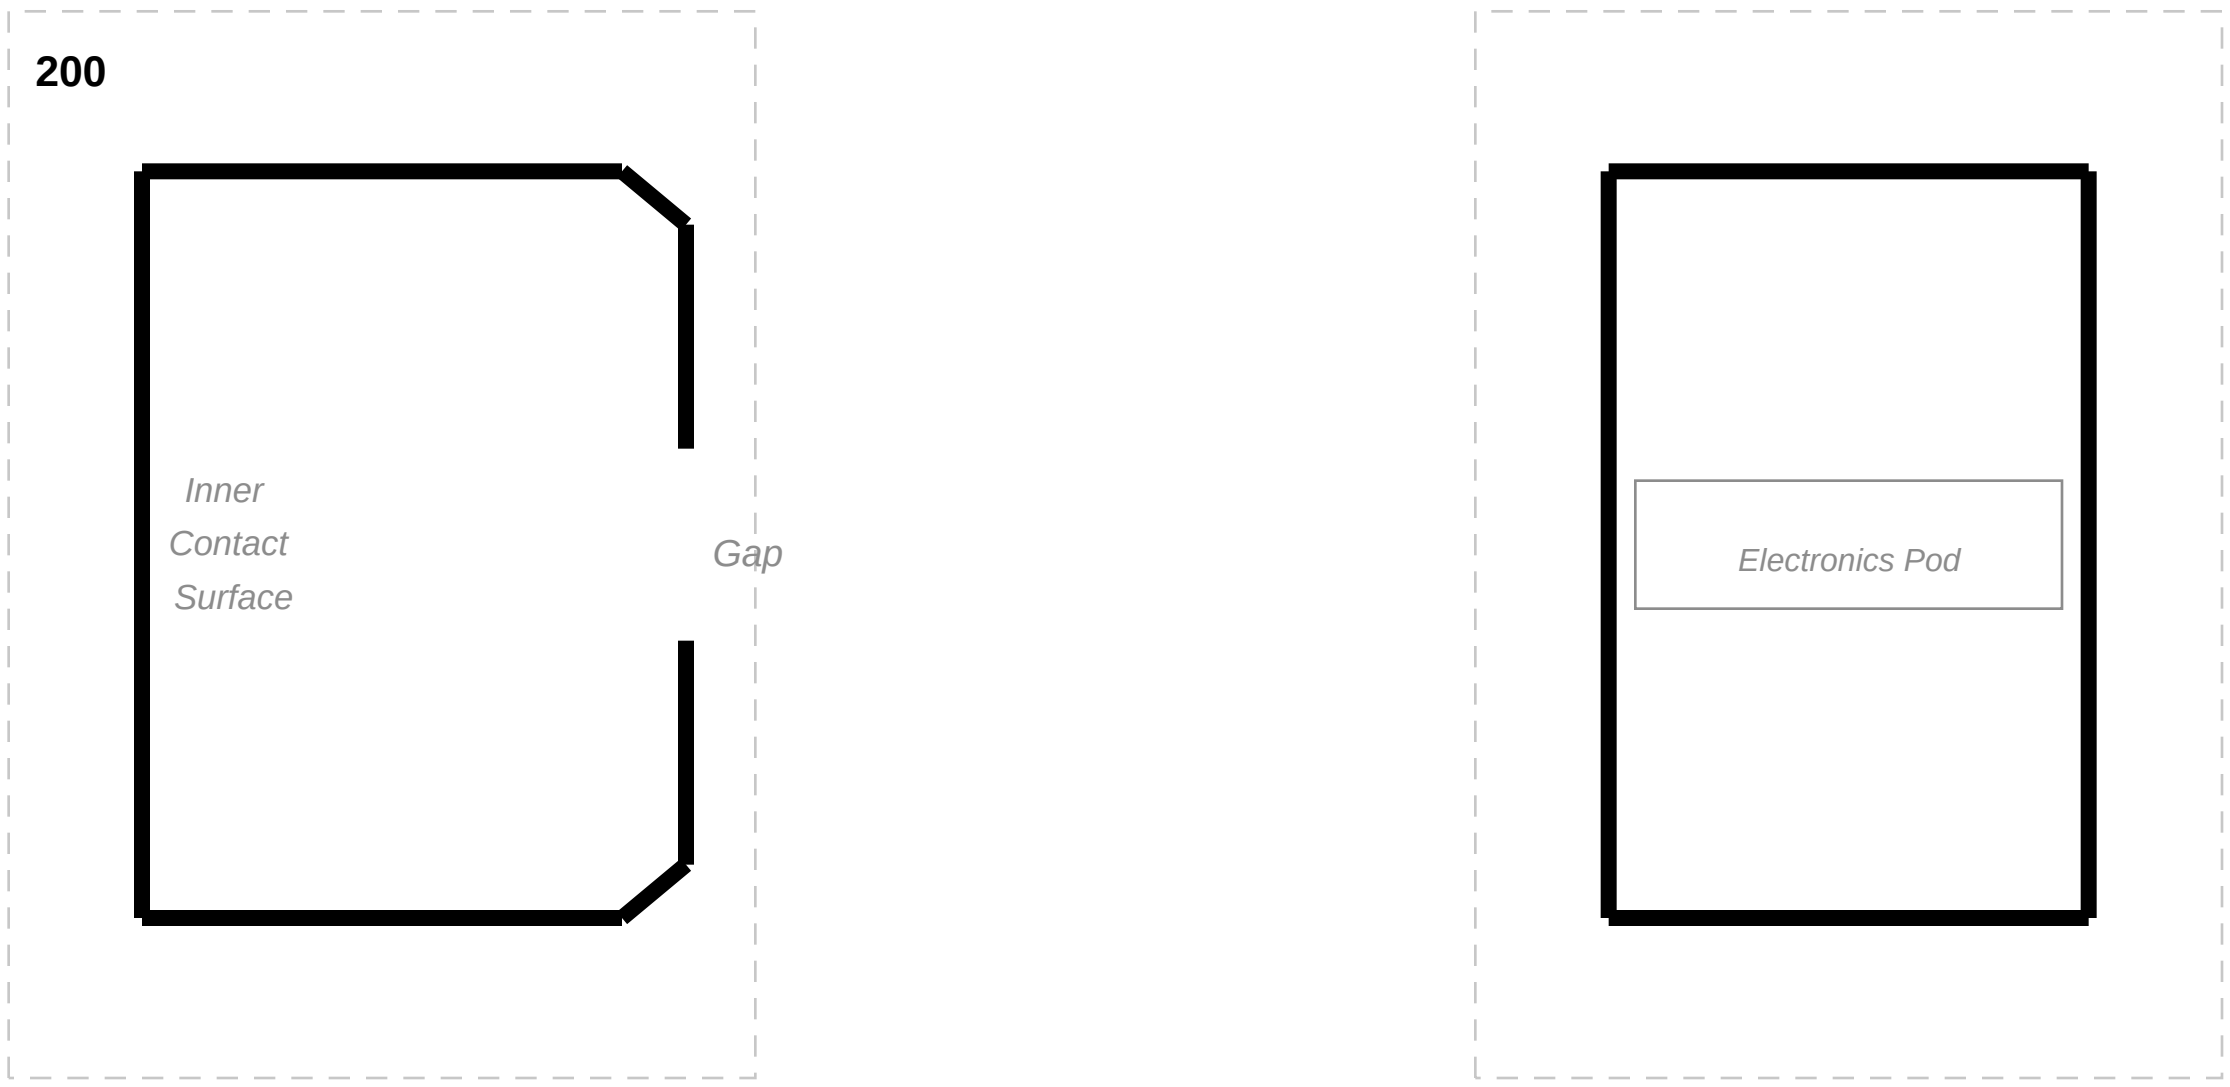

Sensor Suite

Ref	Sensor Modality	Implementation
201	Pressure / Contact Sensors	FSR, capacitive, piezoresistive arrays
202	Strain / Deformation Sensors	Strain gauges, elastomer-embedded elements
203	Hall-Effect Sensor + Magnet	Relative displacement, geometry changes
204	Optical PPG Sensor	Physiologic confirmation, vascular features
205	Temperature Sensor	Thermal context, on-body confirmation
206	6-Axis IMU	Motion gating, orientation, artifact rejection
207	BLE Radio Module	Secure data sync to computing system 110

Output: Privacy-Preserving Metrics

(Indices, Zones, Trends, Confidence -- No Raw Data)

FIG. 3

Node 2 -- Intravaginal Longitudinal Physiology Monitor

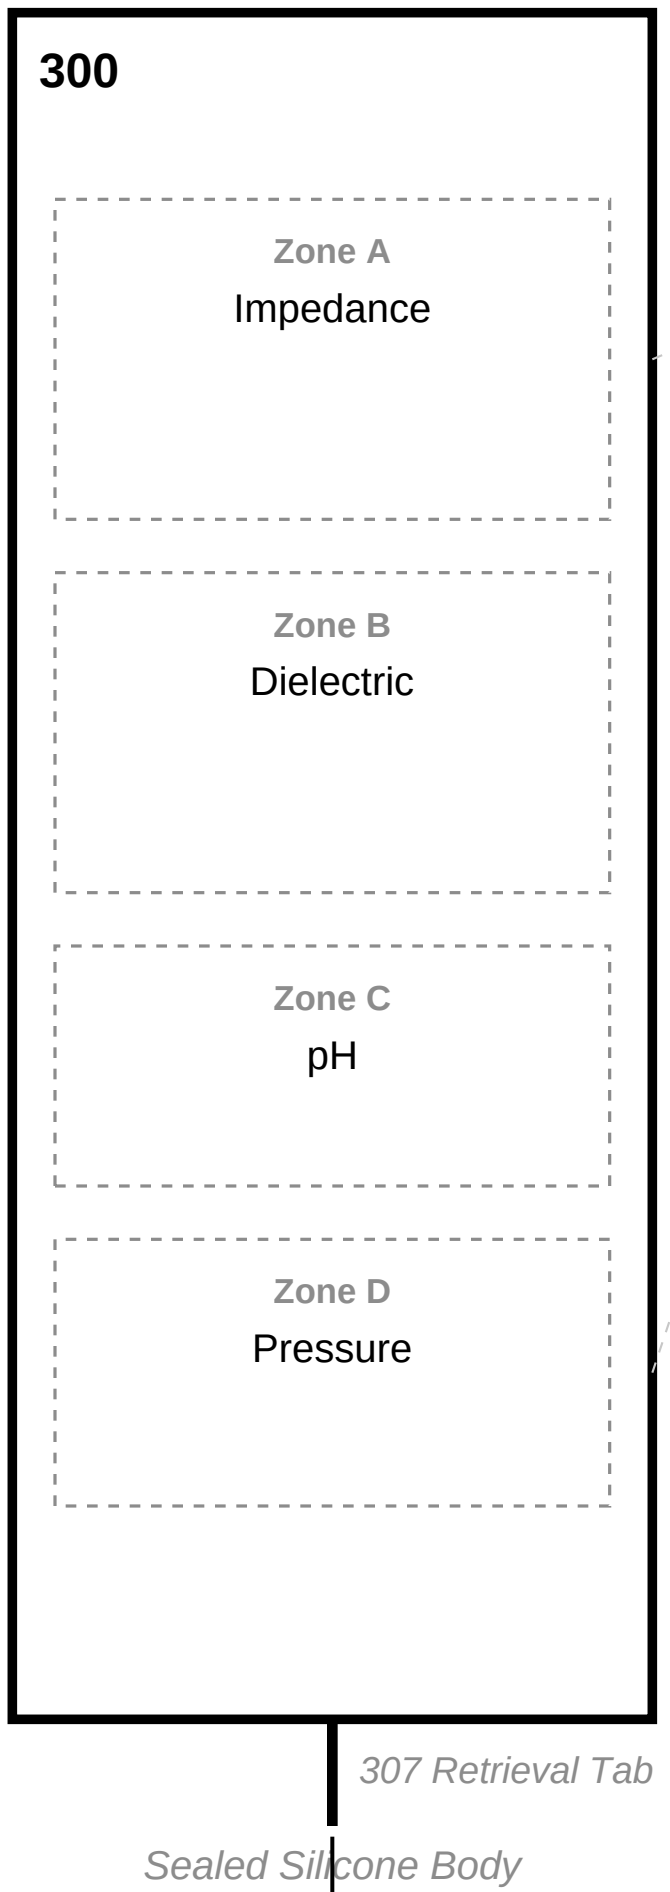

Sensor Suite

Ref	Sensor Modality	Implementation
301	Bio-Impedance Electrodes	Multi-freq., 2-/4-electrode configs
302	Capacitive Wetness / Dielectric	Trend estimation, dielectric changes
303	Solid-State pH (ISFET)	Drift modeling, stabilization routines
304	Distributed Pressure Zones	Multi-zone pelvic activity sensing
305	Temperature Sensors	Context, compensation, placement check
306	6-Axis IMU	Motion gating, orientation, artifacts
307	Retrieval Feature	Sealed tab or retrieval loop

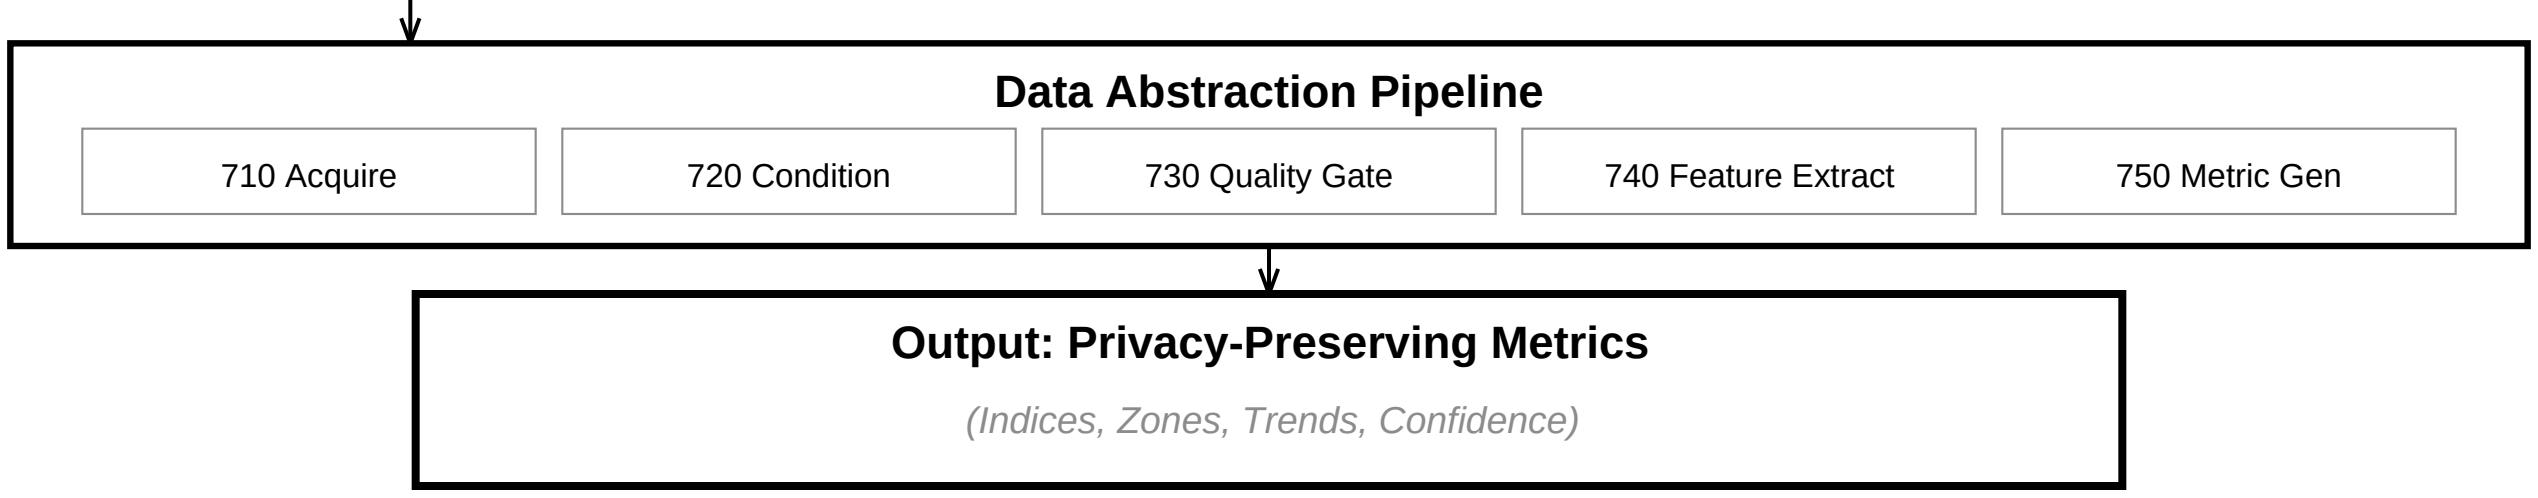

No raw physiological or anatomical data is output by the device.

FIG. 4

Node 3 -- External Geometry Self-Scan Device

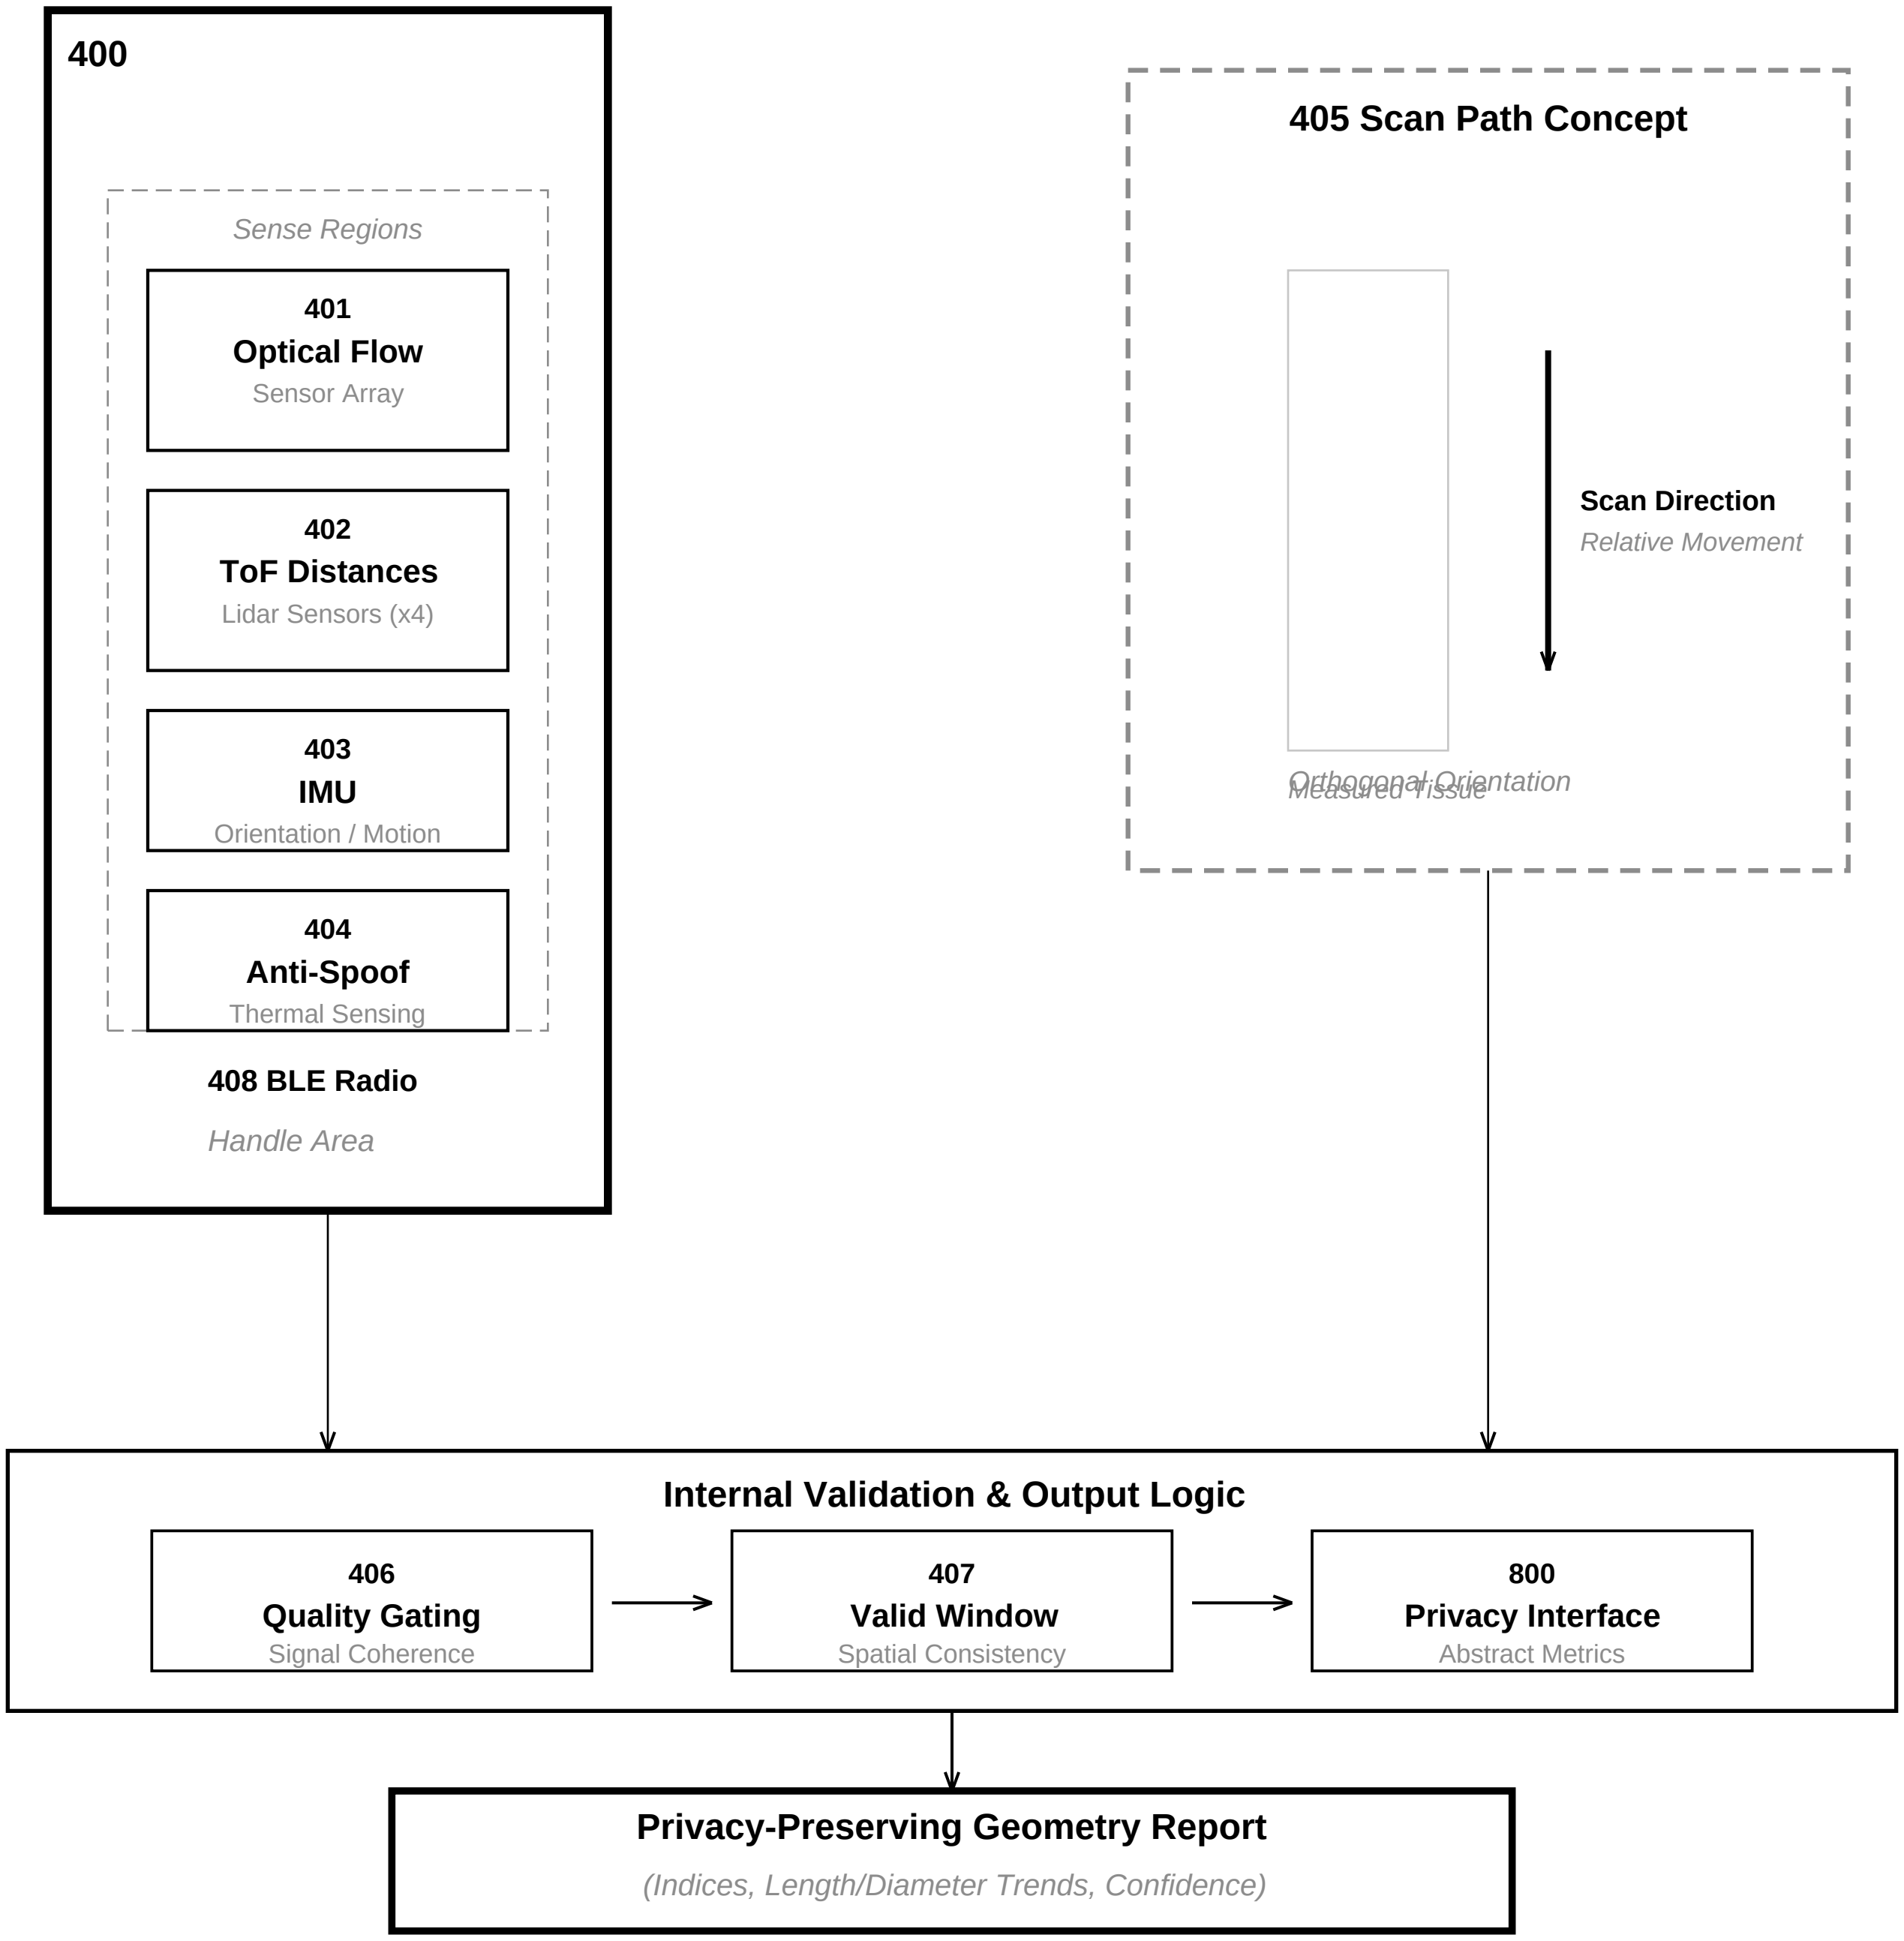

No raw images or anatomical silhouettes are stored or transmitted.

FIG. 5

Node 4 -- Intraluminal Geometry, Compliance, and Contact Device

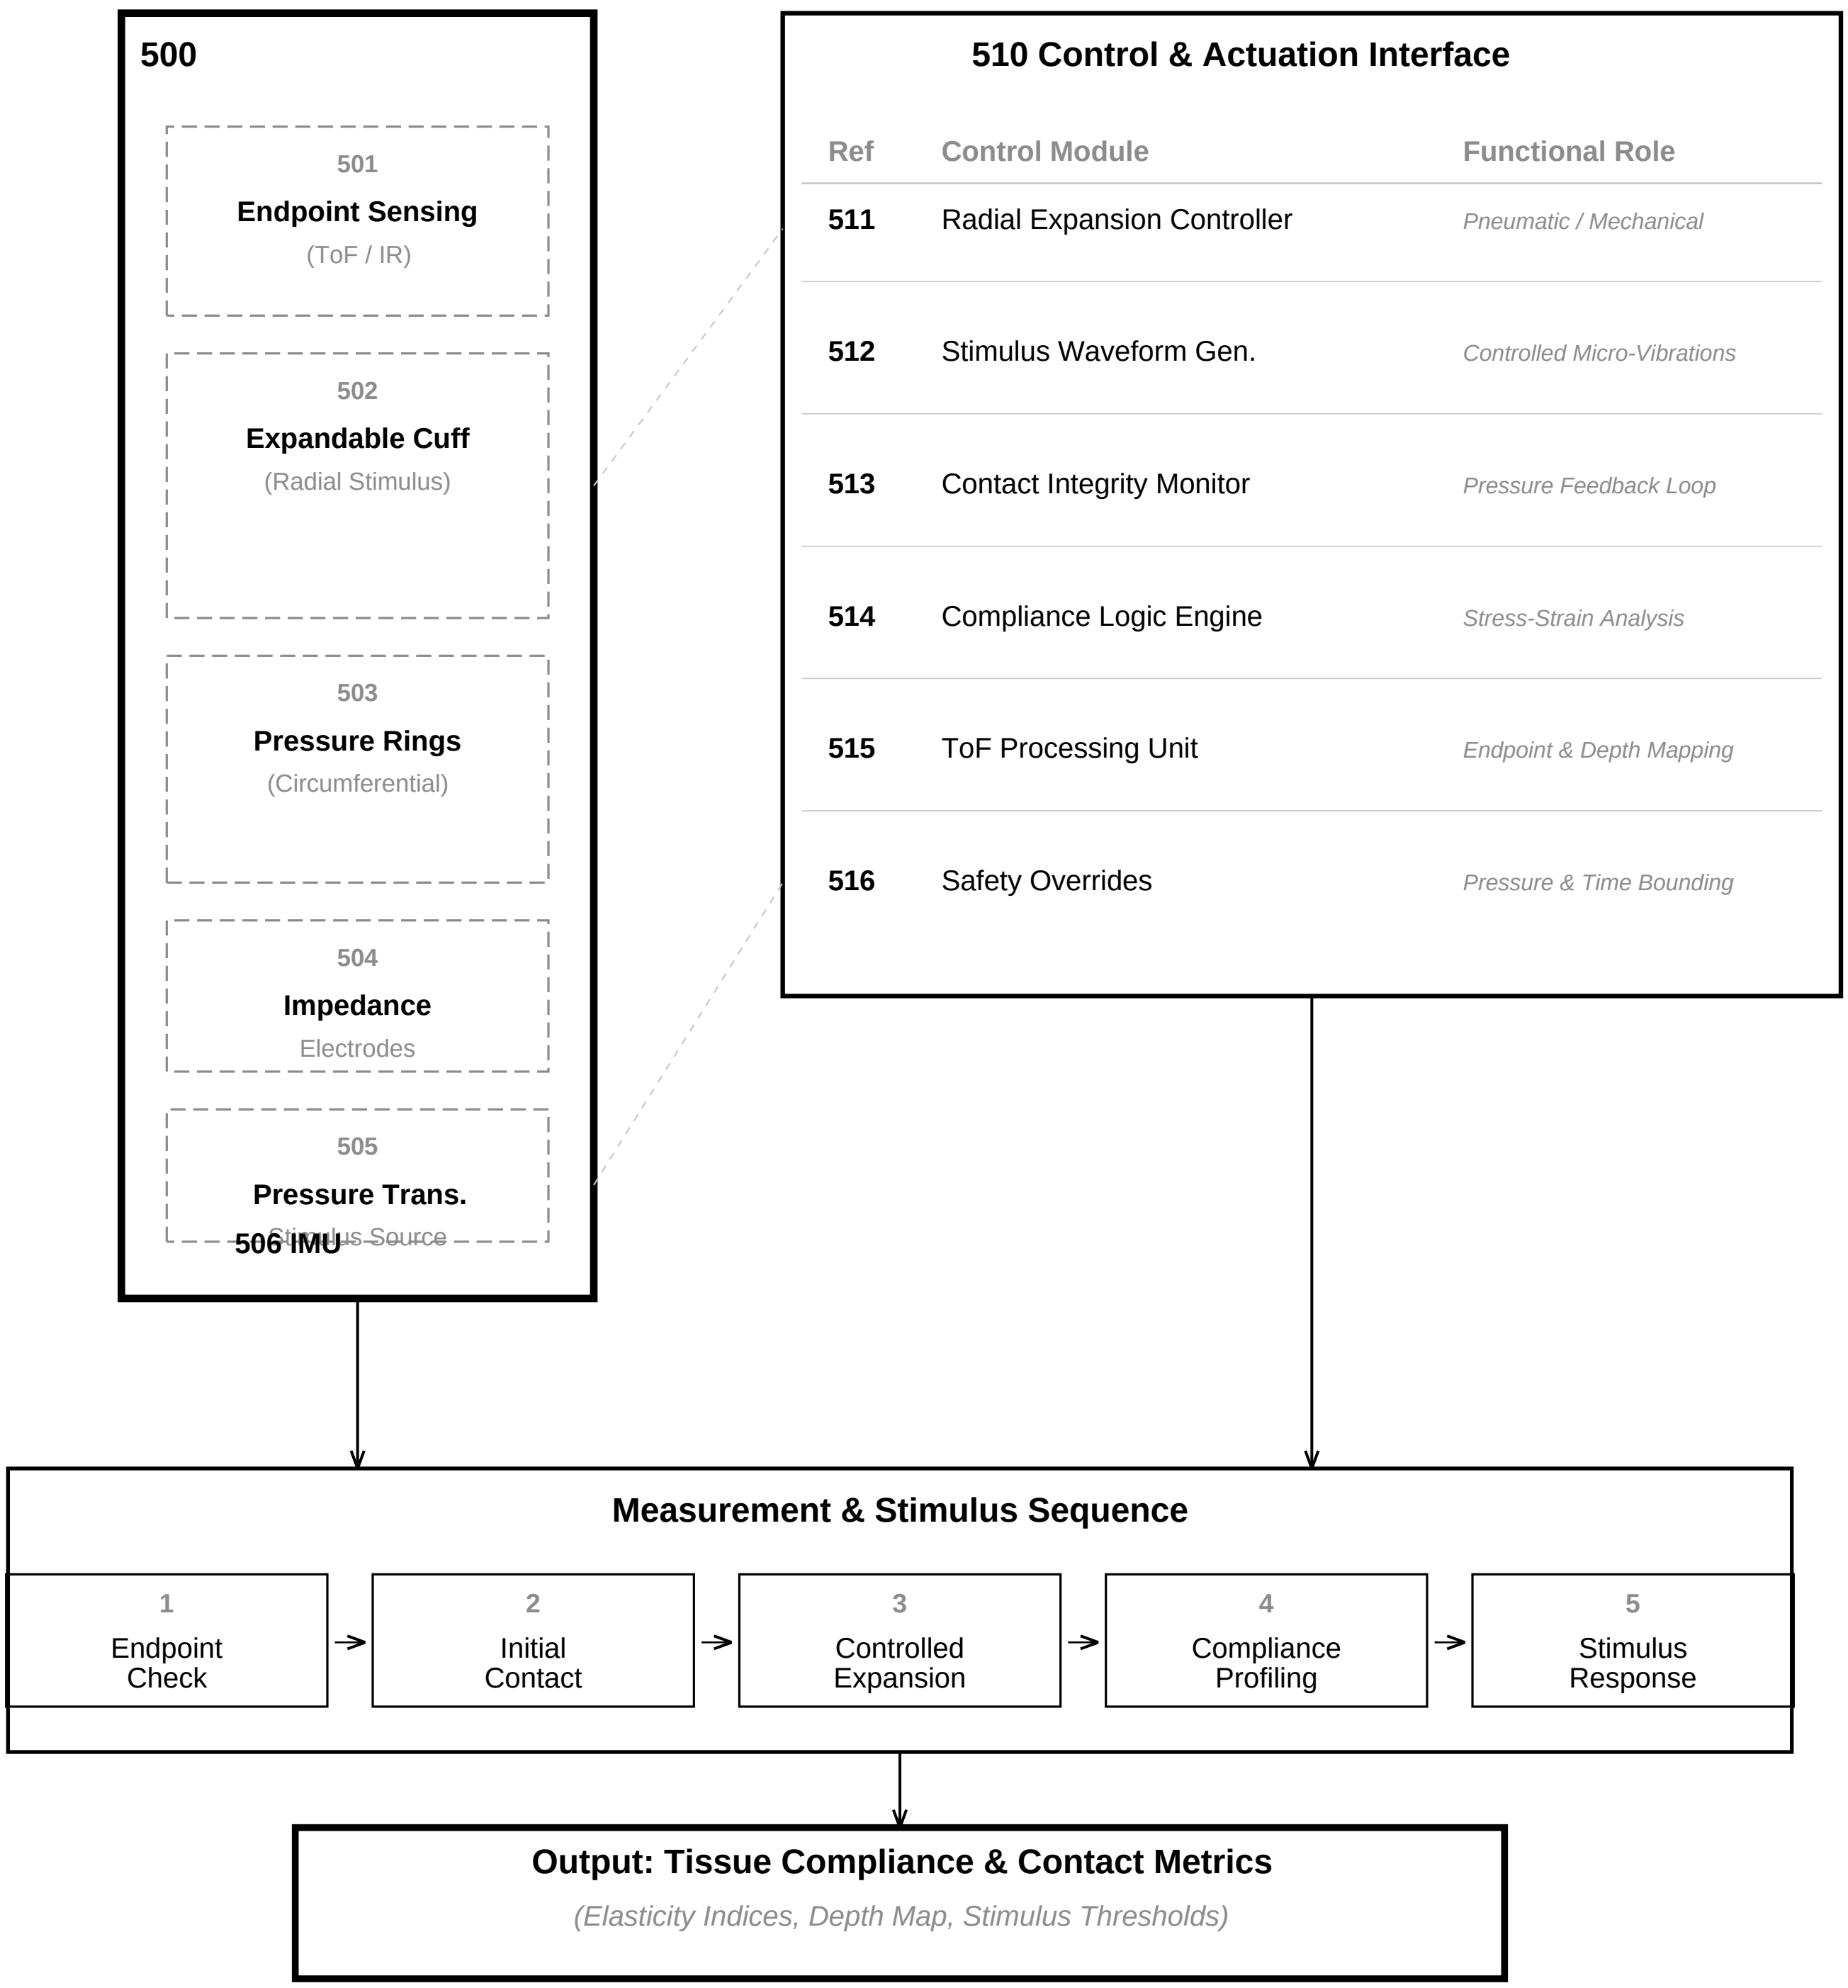

Proprietary non-anatomical sensor abstraction for compliance assessment.

FIG. 6

Node 5 -- Upper-Body Physiologic Context Device

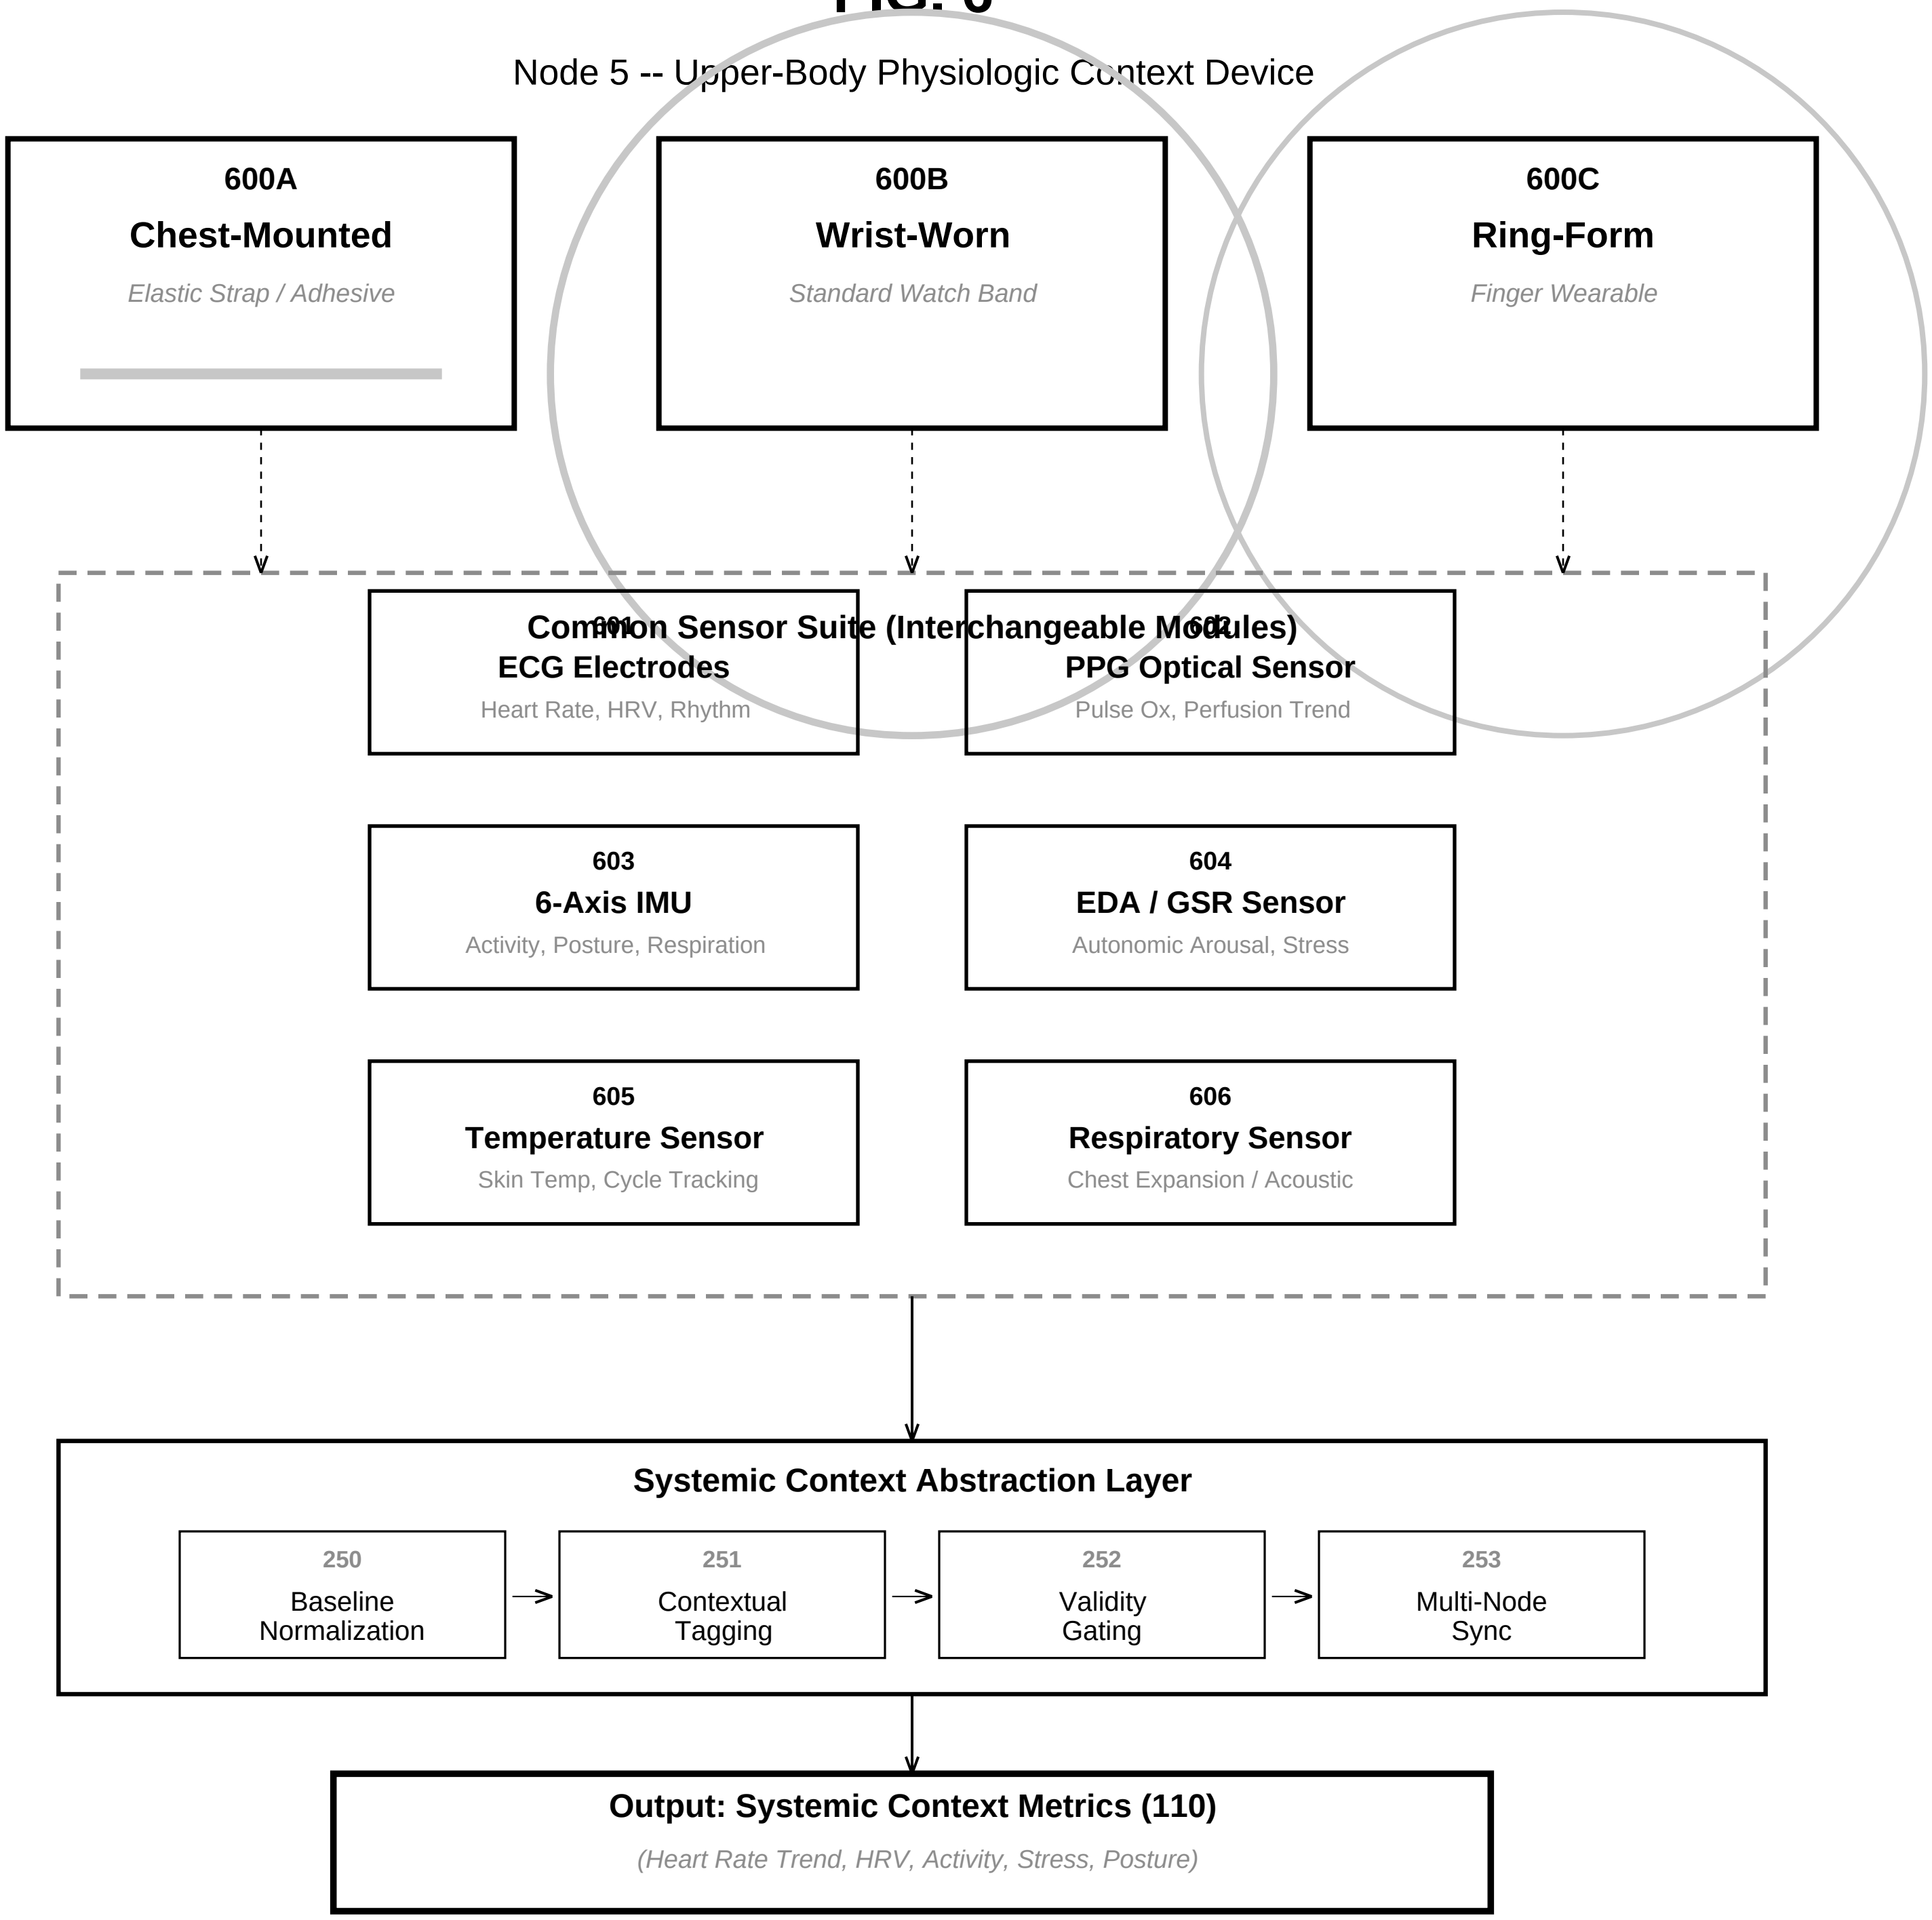

Provides whole-body context to anchor intimate-region measurements.