


FIG. 5

Node 4 -- Intraluminal Geometry, Compliance, and Contact Device

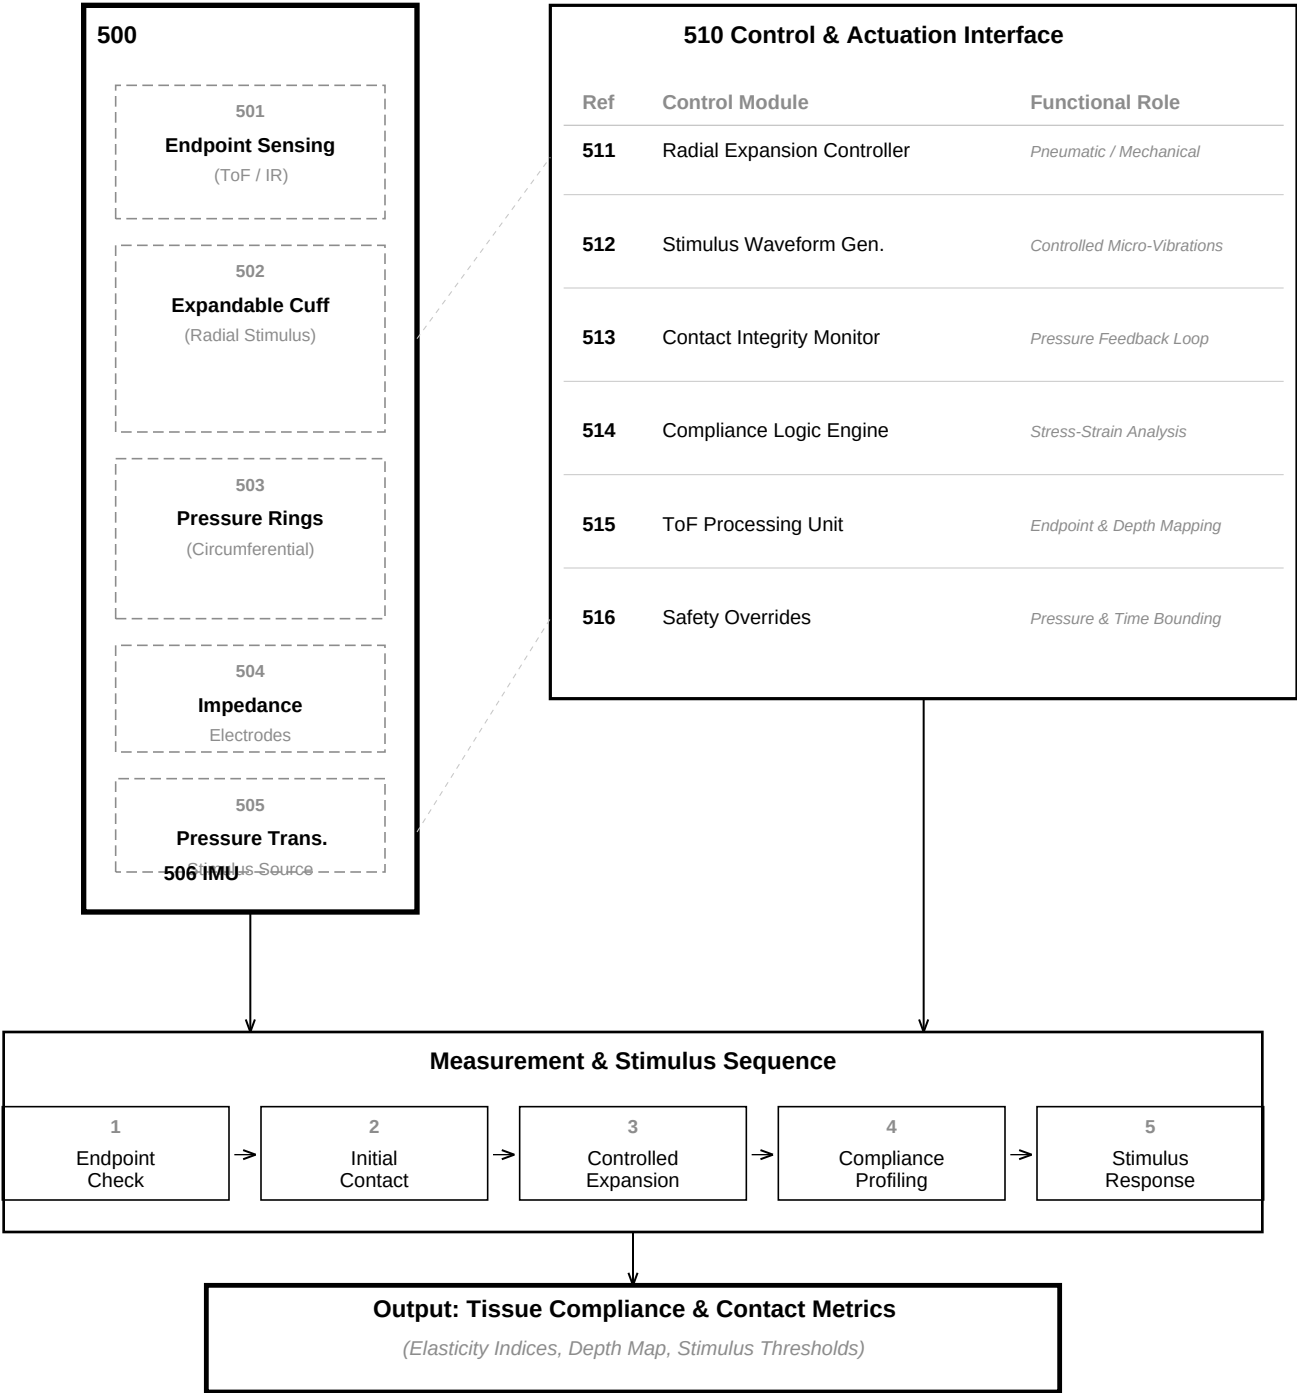

Proprietary non-anatomical sensor abstraction for compliance assessment.