


FIG. 7

Data Pipeline Block Diagram (Acquisition to Reporting)

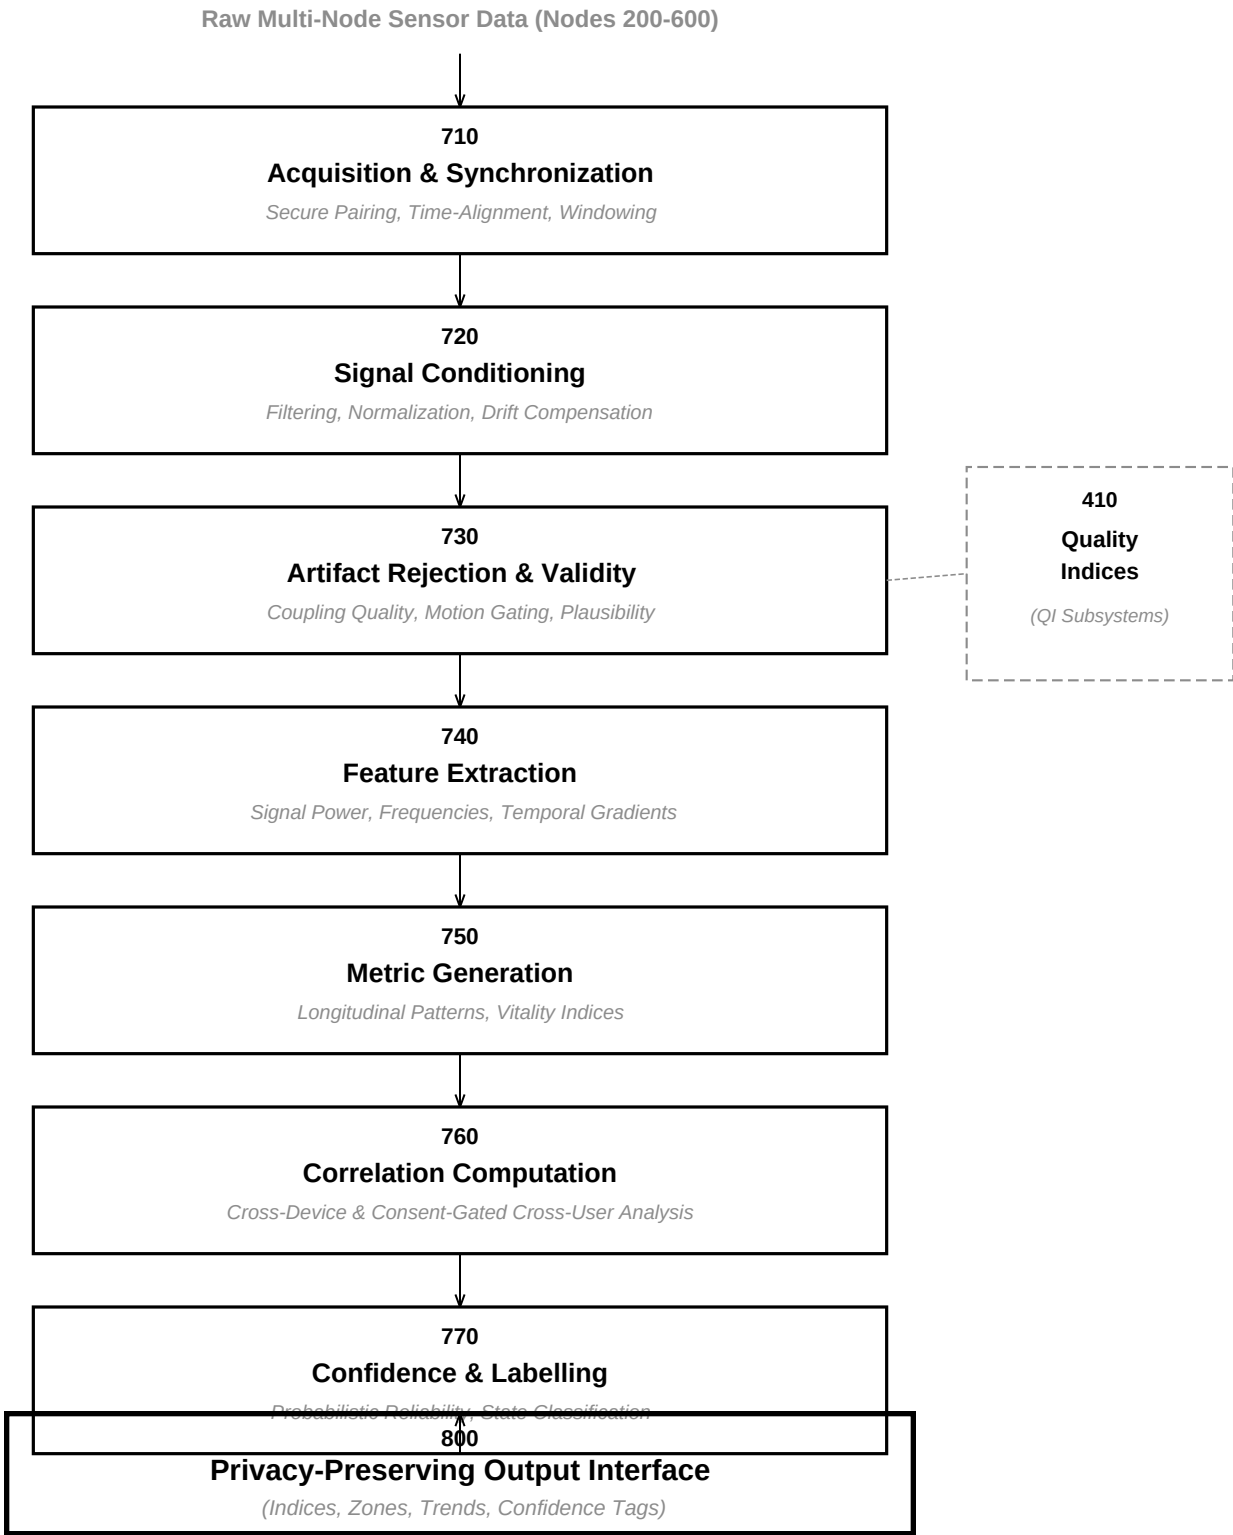

All raw data is discarded post-processing or held in enclave memory.

FIG. 8

Cross-Device Correlation Workflow (Time-Aligned Sensing)

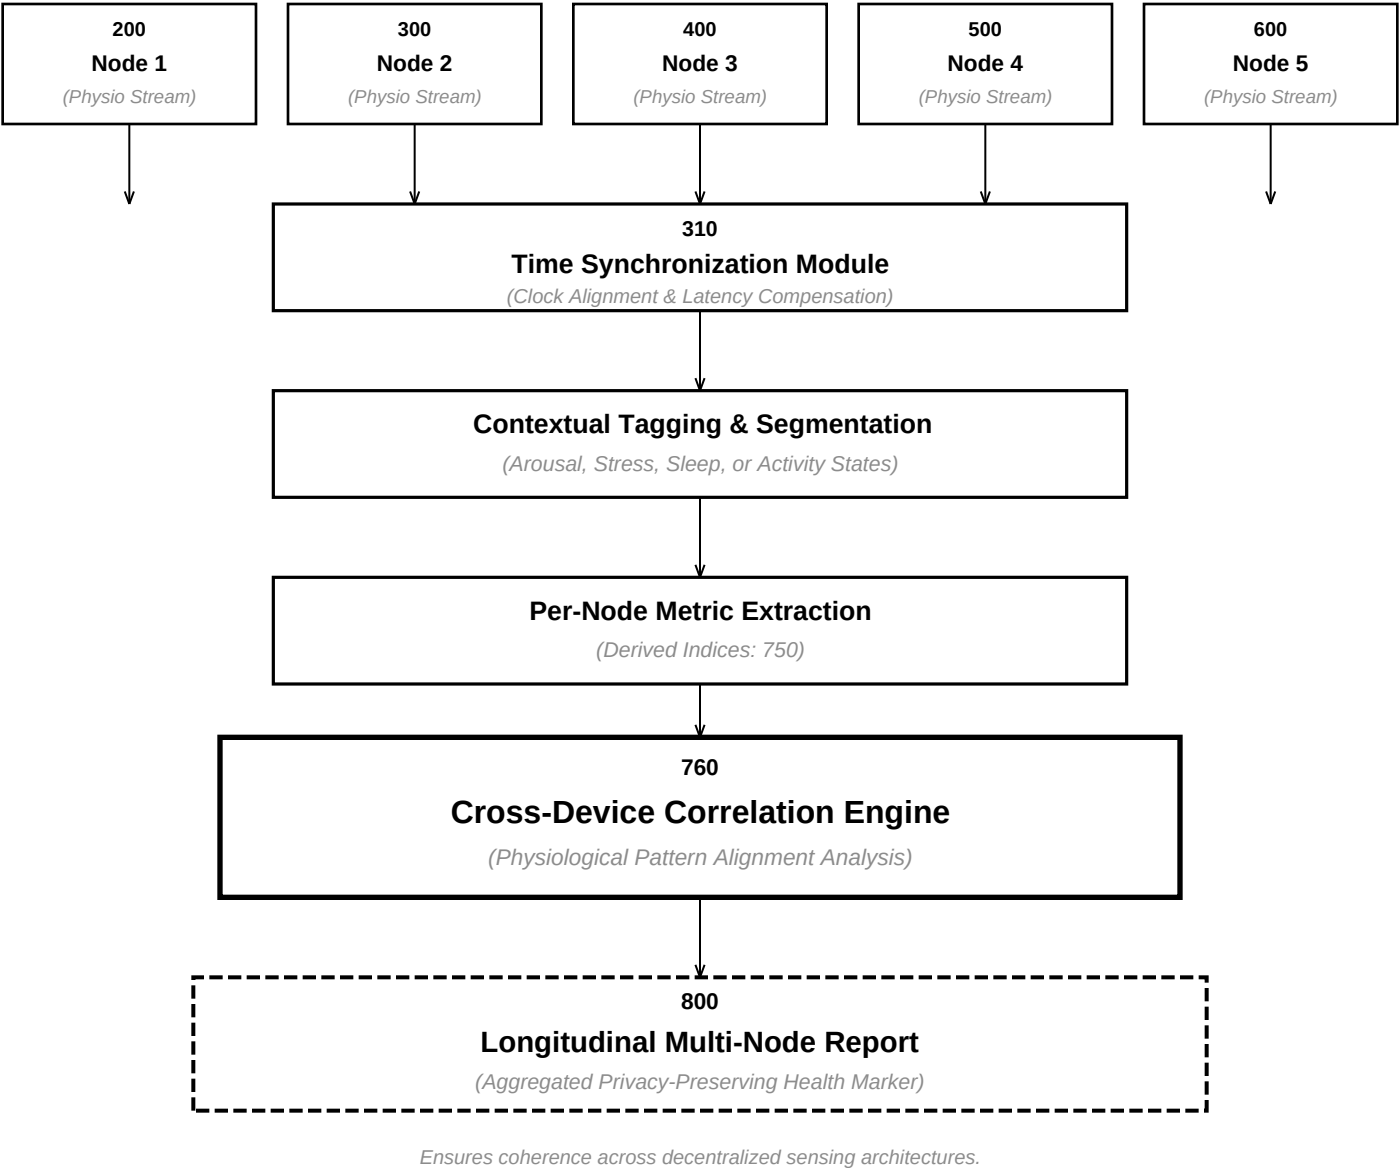


FIG. 9

Cross-User Correlation and Consent-Gated Sharing


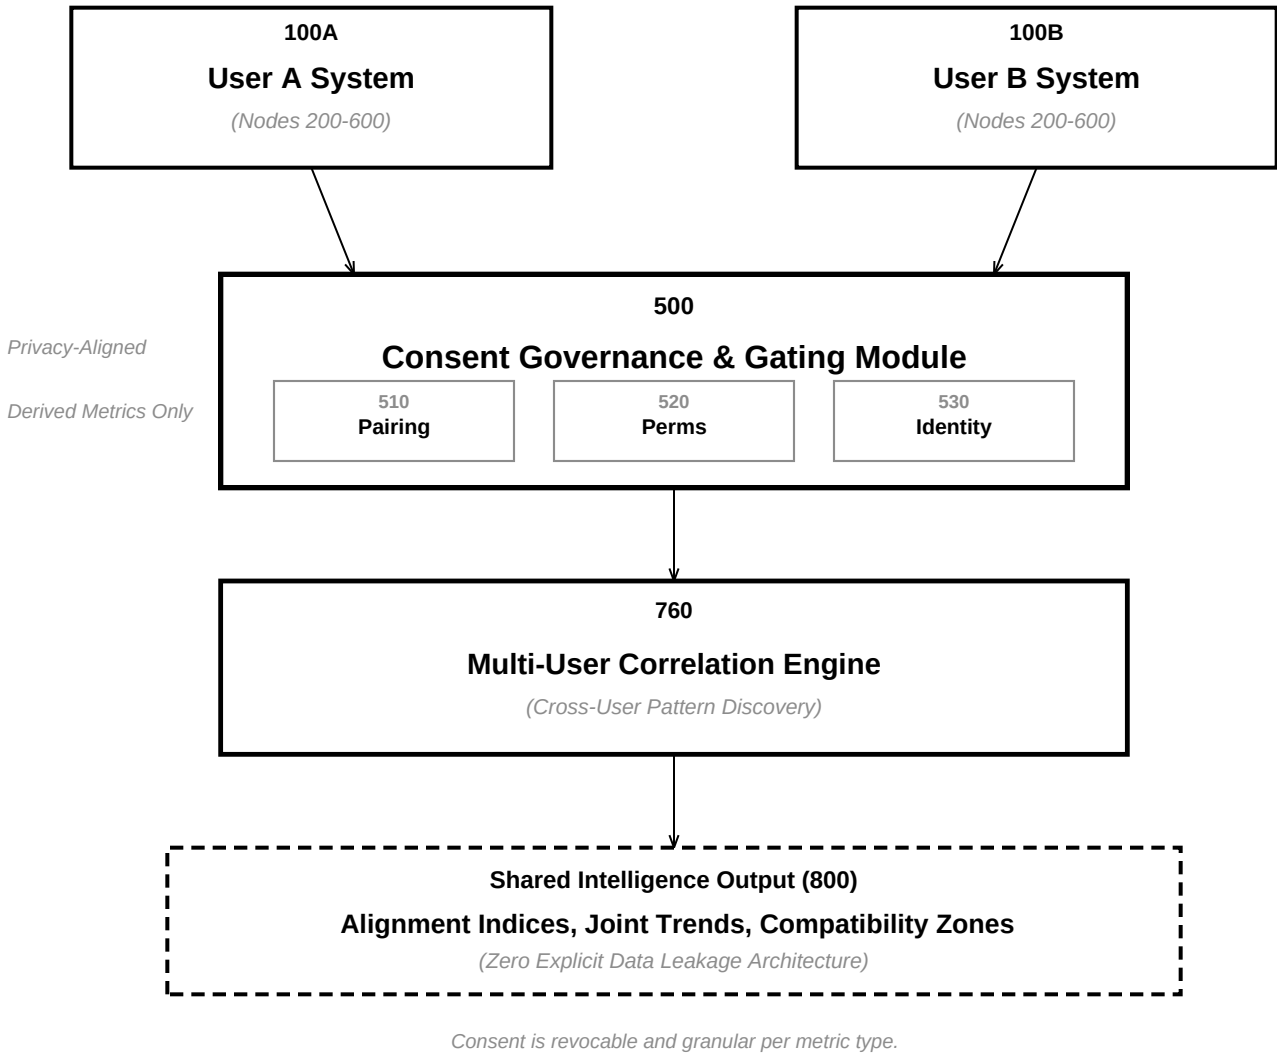


FIG. 10

Privacy-Preserving User Interface (Abstract Metric Representation)

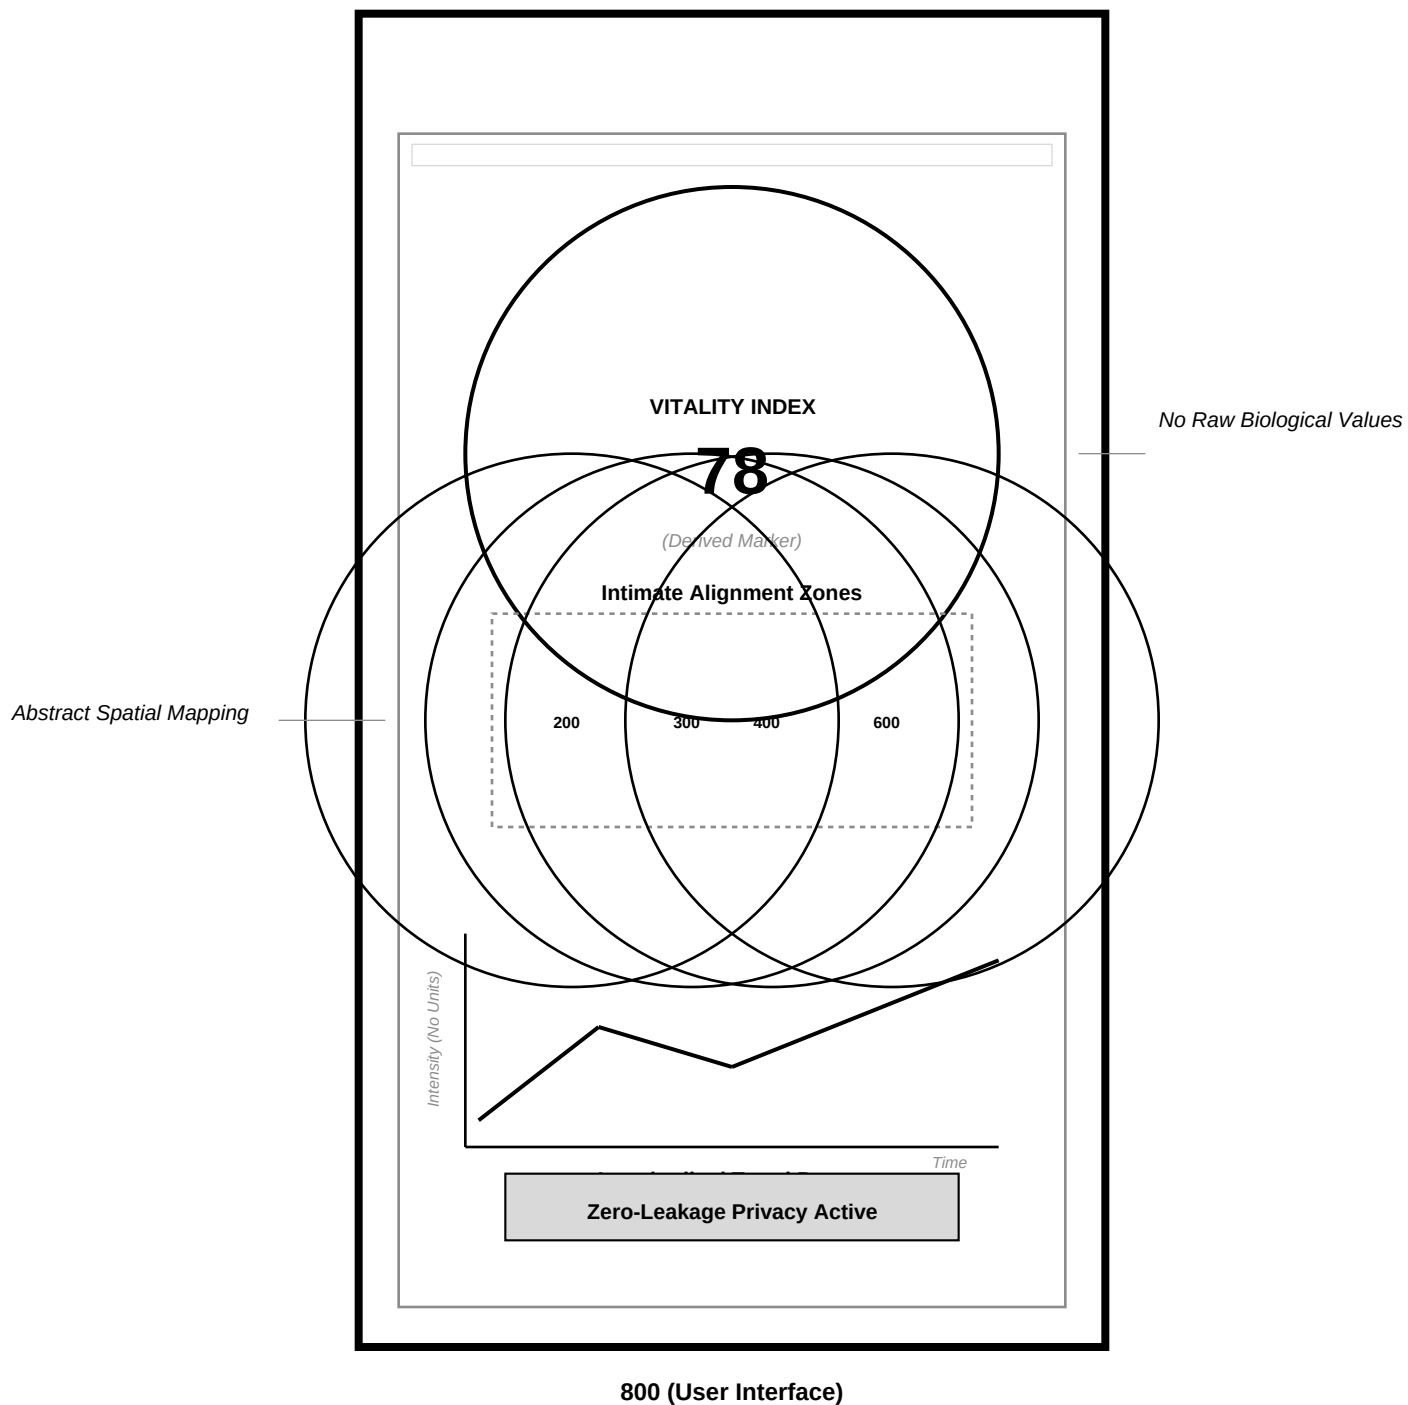

The UI presents computed indices and abstract visualizations rather than explicit physiological data.

FIG. 11

Flexible Multi-Pairing Correlation Topologies



Scenario A: Prototypical Correlation (M-F)



Scenario B: Flexible Gender-Neutral Pairing (M-M, F-F, etc.)




Scenario C: One-to-Many Contextual Correlation

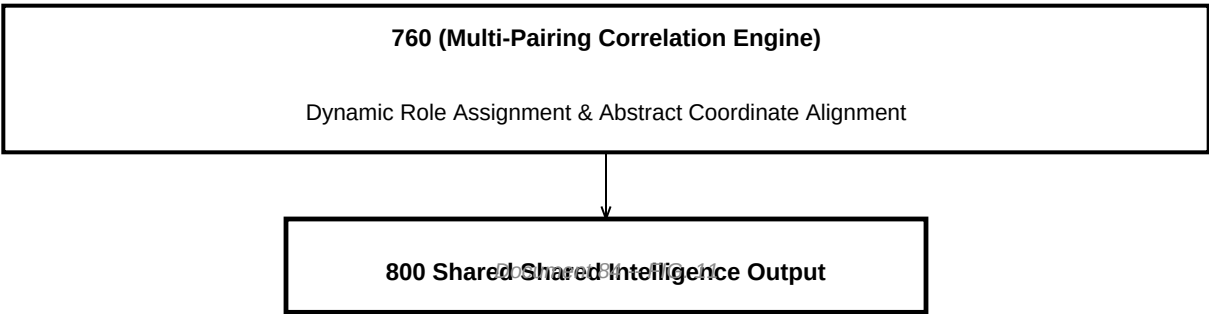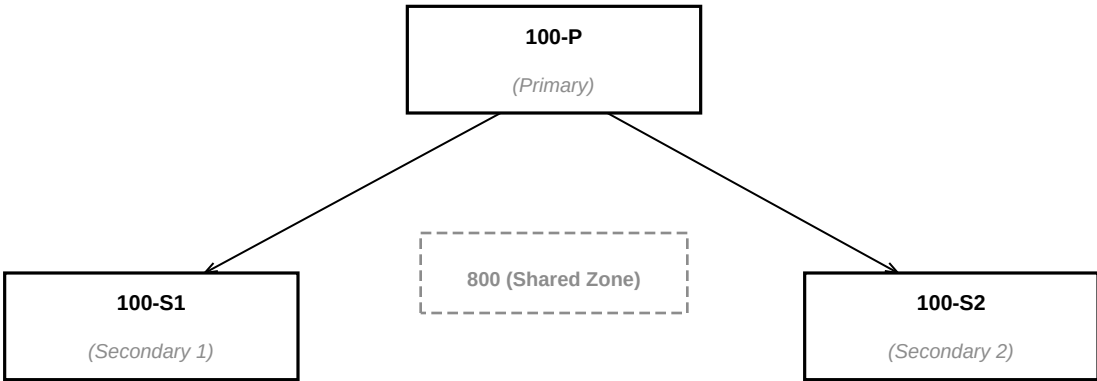

Architecture is gender-agnostic and supports arbitrary n-way pairing via consent governance.

FIG. 12

End-to-End System Workflow (Lifecycle of a Session)

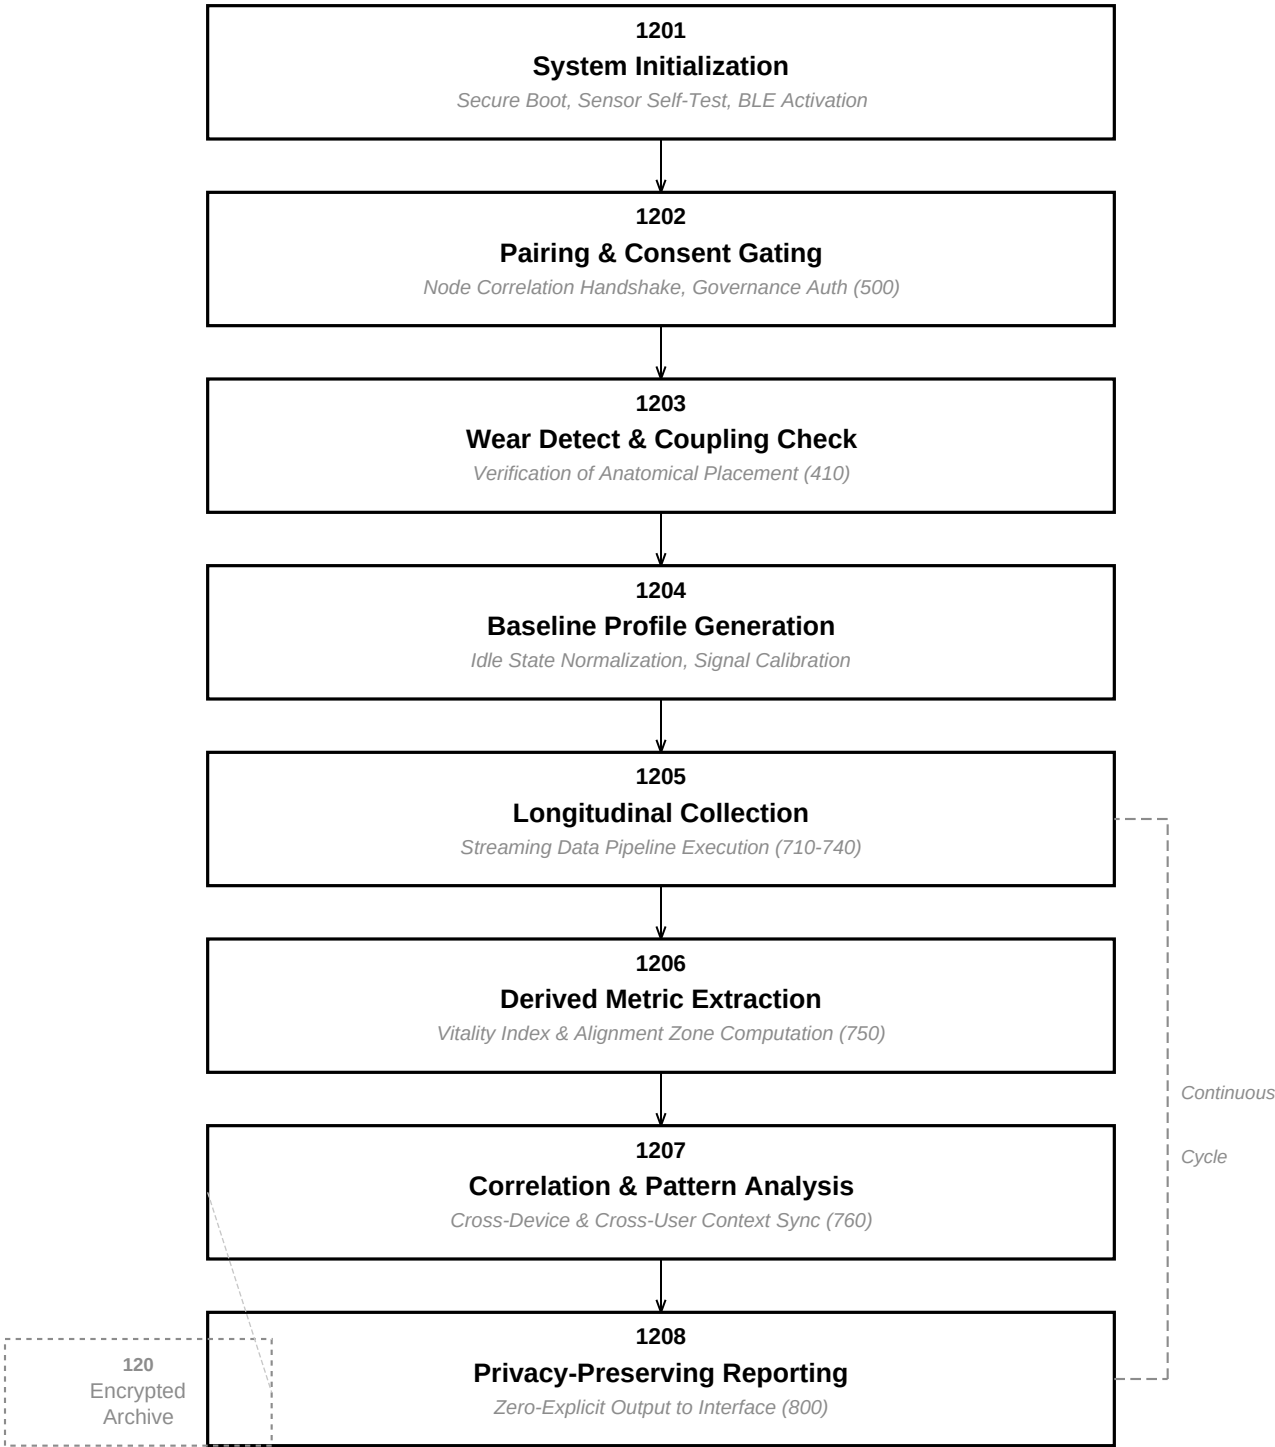

Chronological sequence of operations for an active Nexalis Health session.