

FIG. 1

High-Level Block Diagram of Multi-Node Monitoring System

100 System

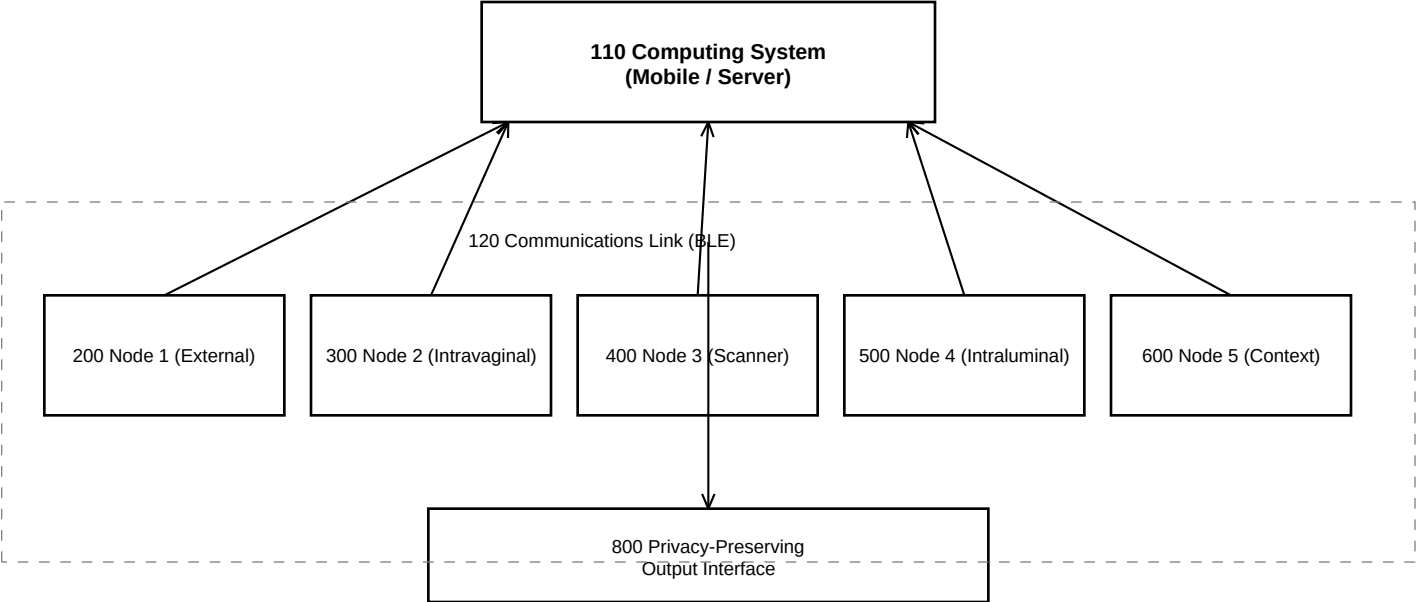


FIG. 2

Example Data-Flow Diagram (Privacy-Preserved)

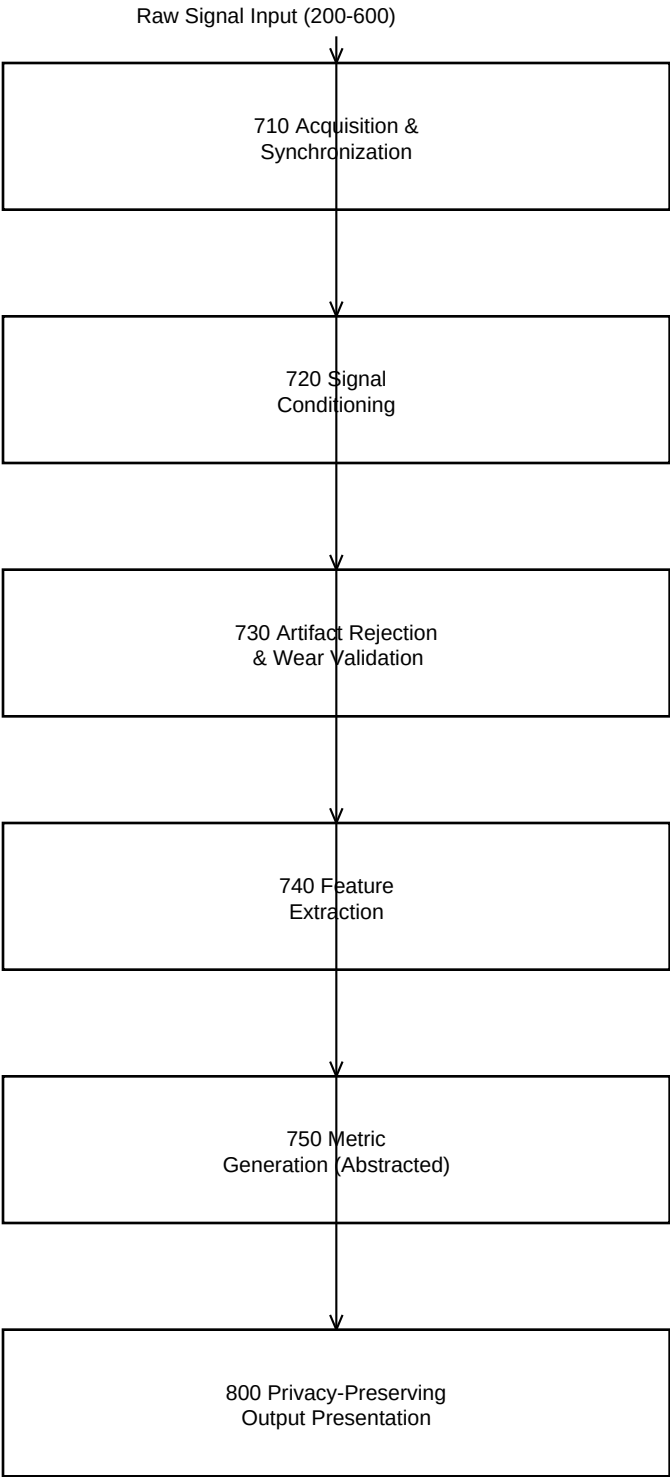


FIG. 3

Cross-Device Correlation between Intimate and Context Nodes


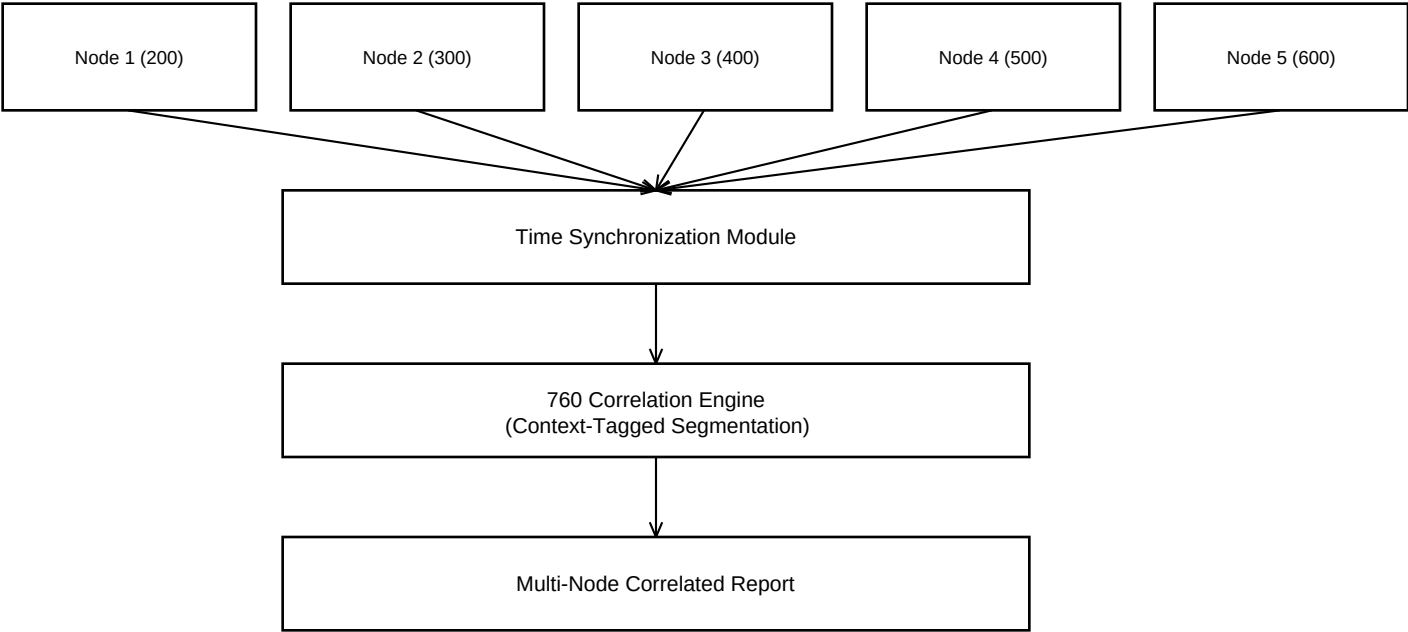


FIG. 4
Baseline Establishment and Longitudinal Tracking

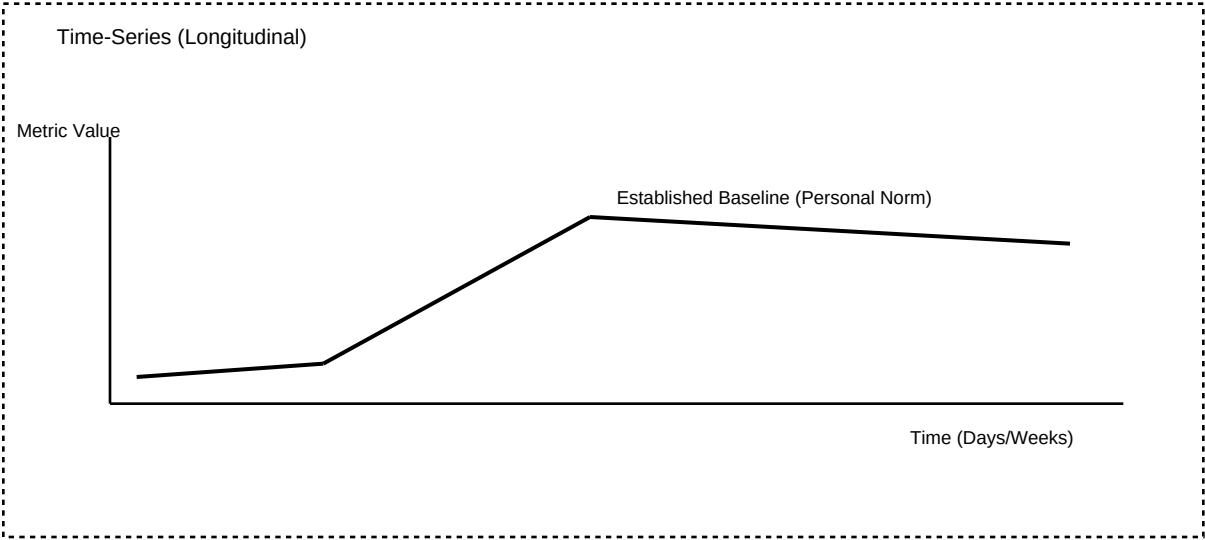

Baseline Establishment
(Initial Calibration Window)

Window Comparison
(Trend Analysis vs Baseline)

Confidence Indicator
(Data Quality Gate)

FIG. 5

Node 1 — All-Day/Night External Tumescence and Rigidity Monitor

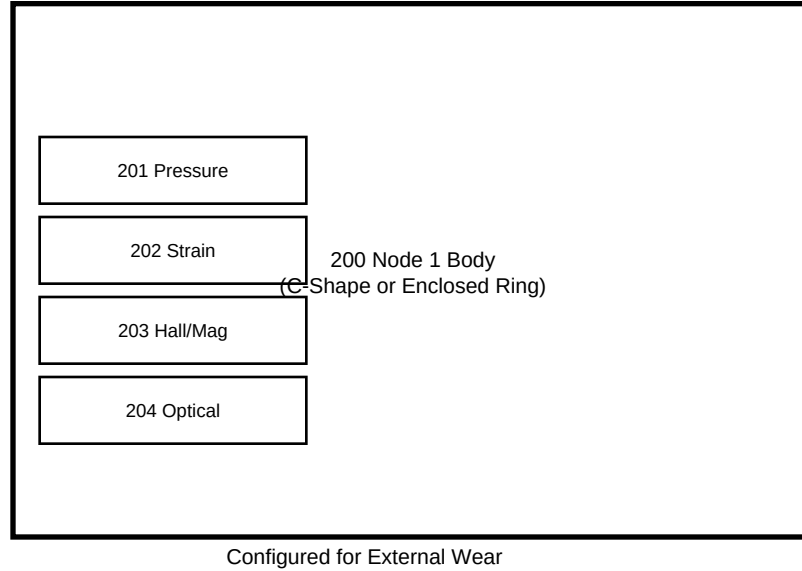


FIG. 6

Node 2 — Intravaginal Longitudinal Physiology Monitor


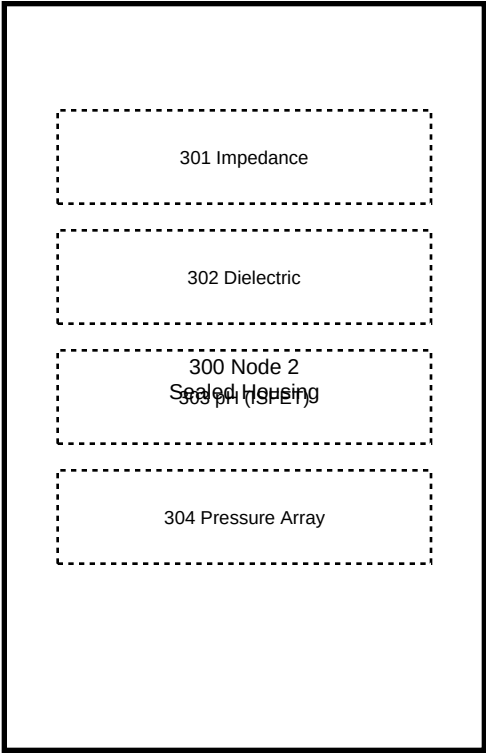


FIG. 7


Node 3 — Self-Scan External Geometry Measurement Device

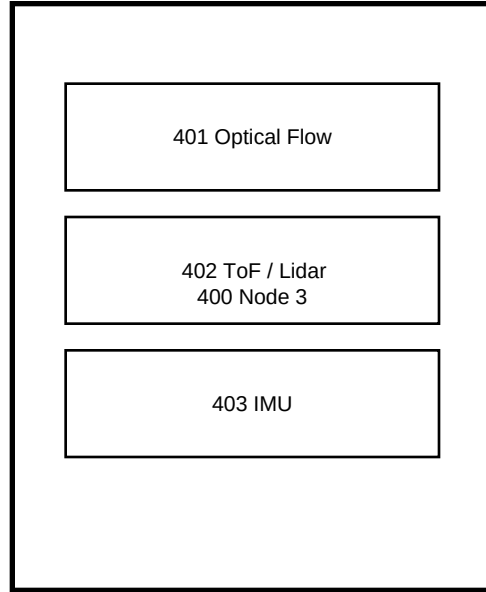

Measurement Path Validation

FIG. 8

Node 4 — Intraluminal Geometry, Compliance, and Contact Device

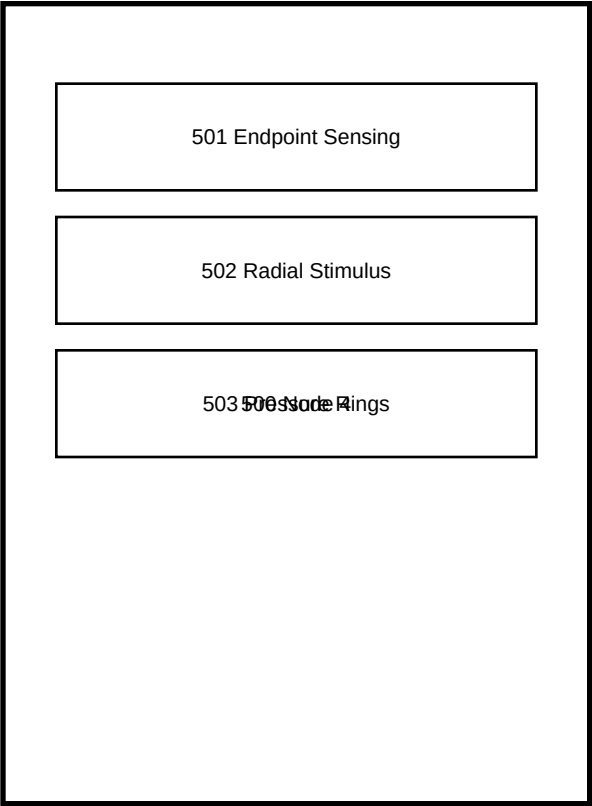

Controlled Internal Measurement

FIG. 9

Node 5 — Upper-Body Physiologic Context Device

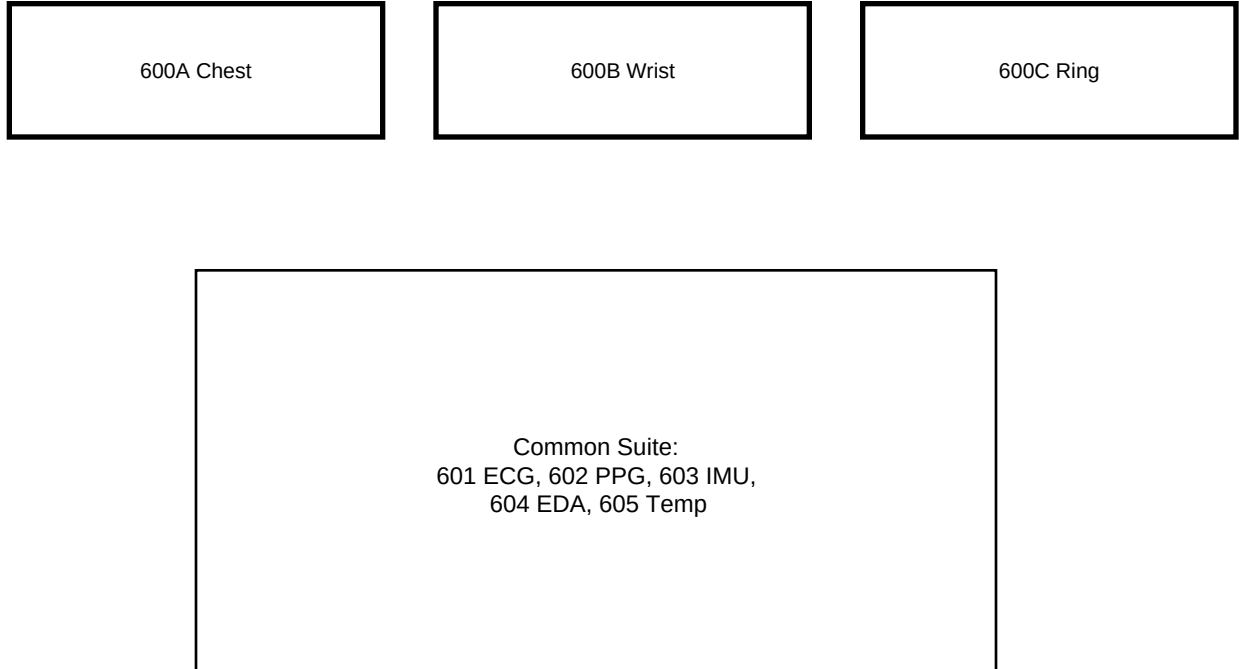


FIG. 10

Privacy-Preserving User Interface Output

- Vitality Index (Non-Numeric)
- Sigil Representation
- Pattern Curves (Longitudinal)
- No Anatomical Imagery

800 Output Interface Mockup

FIG. 11

Privacy-Preserving Cross-User Correlation

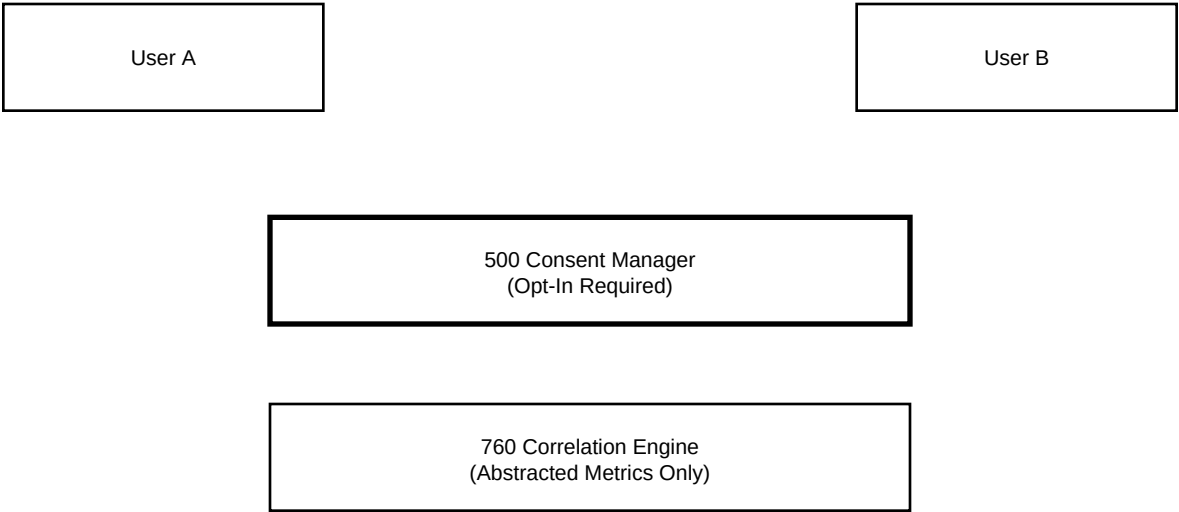


FIG. 12

System Workflow: Initialization to Longitudinal Correlation

