


FIG. 3

Node 2 -- Intravaginal Longitudinal Physiology Monitor

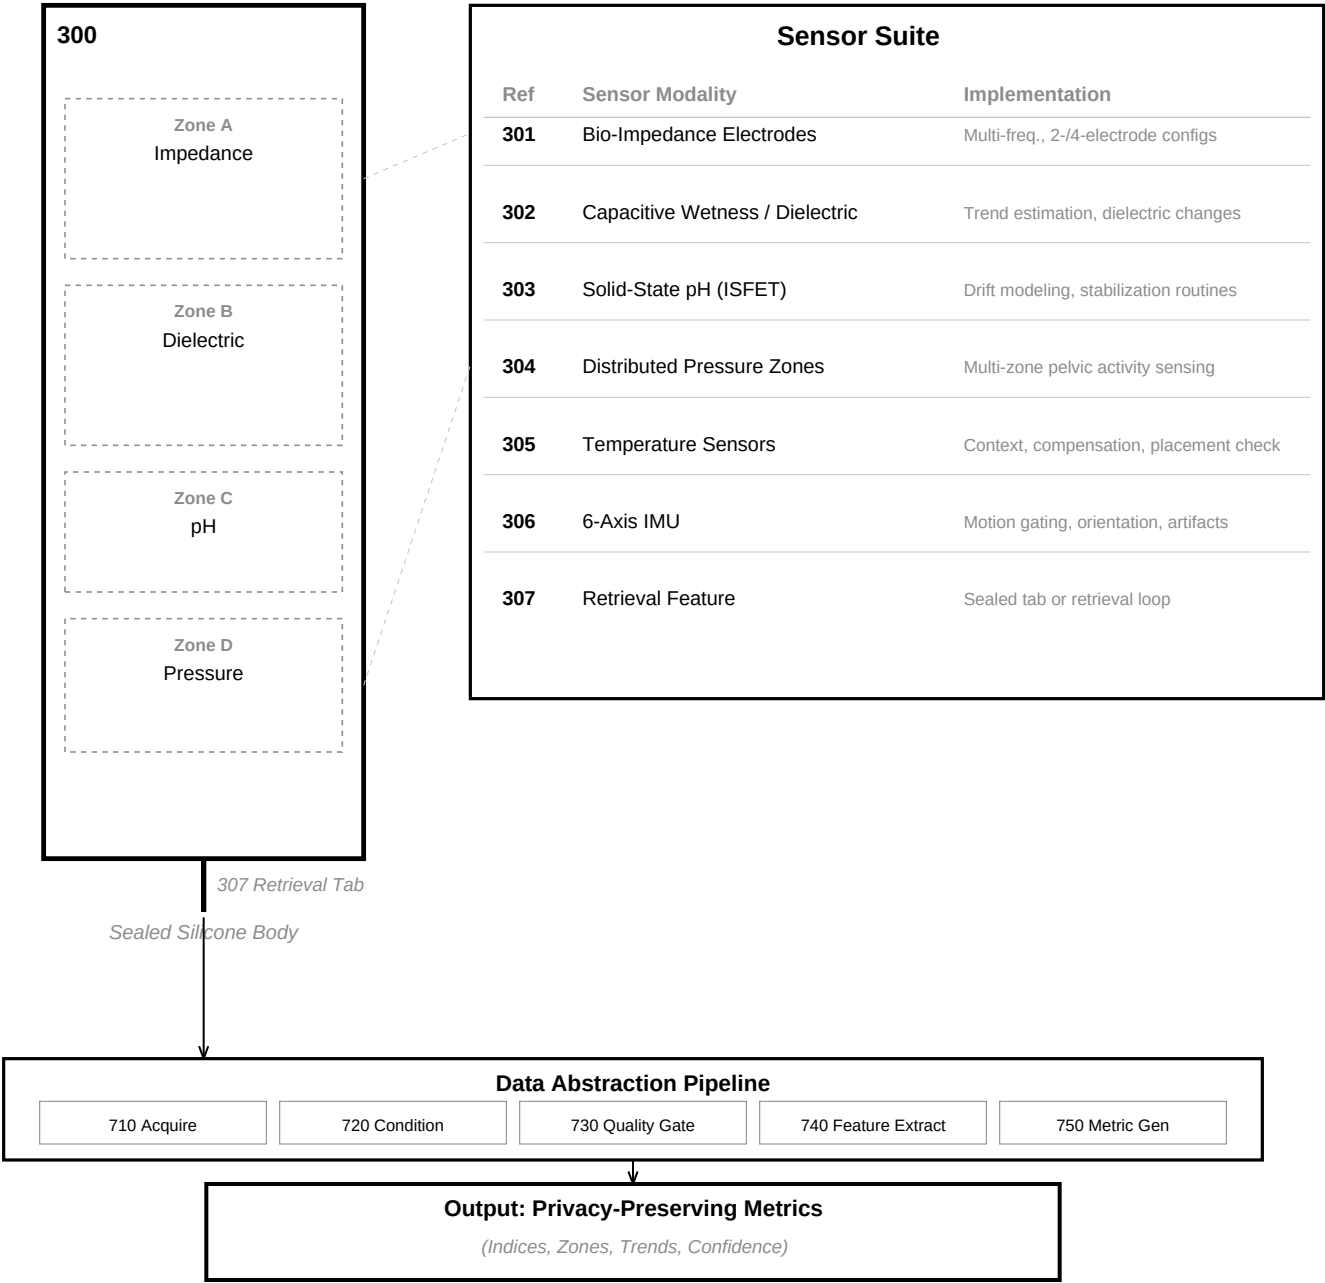

No raw physiological or anatomical data is output by the device.