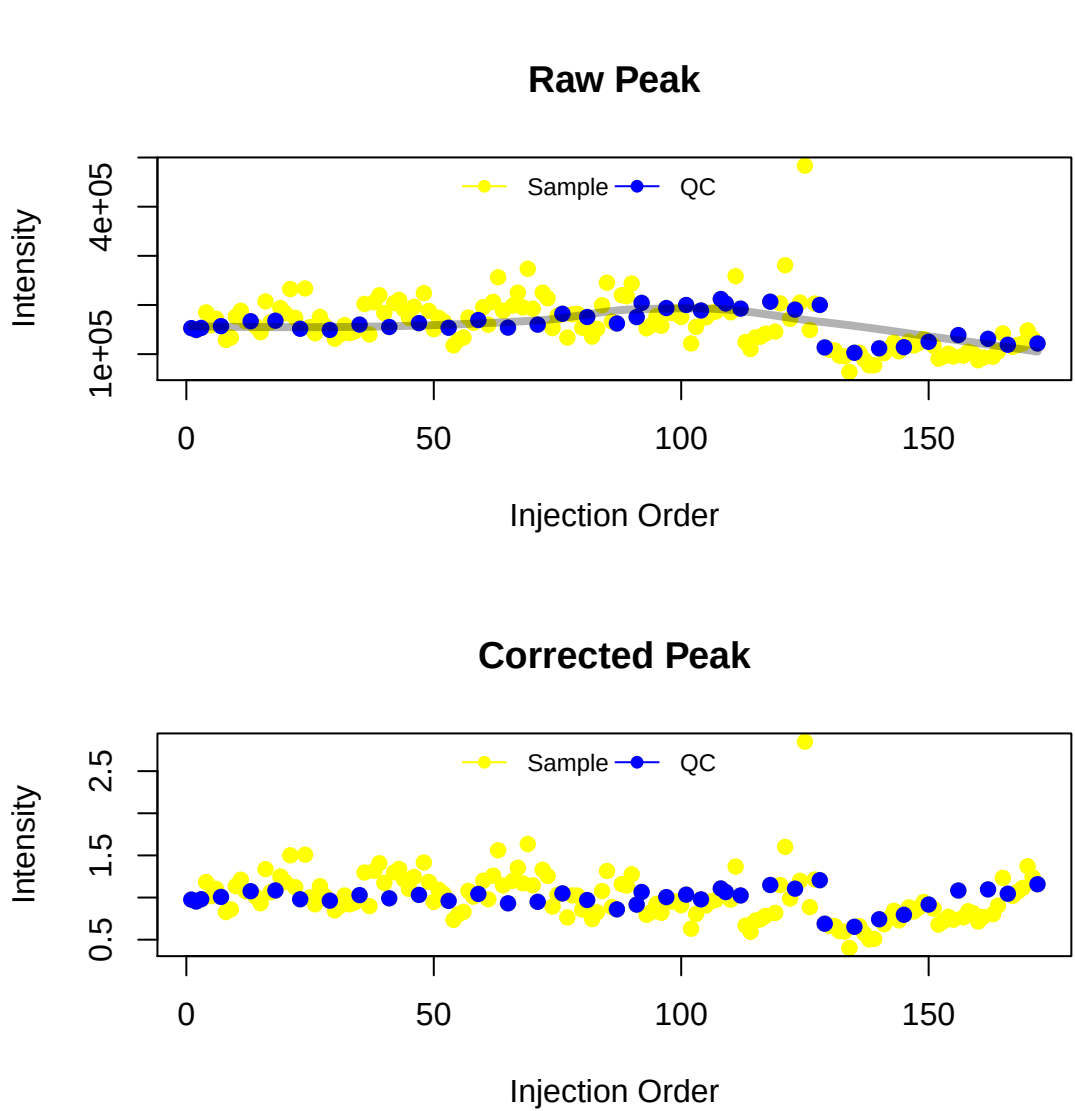
Raw Peak
Intensity
1e+05
4e+05
Sample
QC
0
50
100
150
Injection Order
Corrected Peak
Intensity
0.5
1.5
2.5
Sample
QC
0
50
100
150
Injection Order